

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
 Data File : BM016510.D
 Acq On : 22 Aug 2018 08:35
 Operator : SJ/JU
 Sample : J4271-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HR-06-082018-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	381	387	411	rBV	4367076	6467369	11.99%	4.257%
2	7.198	658	665	680	rBV	3709513	5723982	10.61%	3.768%
3	7.551	718	725	740	rBV	5890677	9005818	16.69%	5.928%
4	8.022	795	805	820	rBV	818346	1471813	2.73%	0.969%
5	8.334	851	858	872	rBV	4454310	7267853	13.47%	4.784%
6	9.204	999	1006	1020	rBV	2797586	4733539	8.77%	3.116%
7	10.827	1272	1282	1290	rBV	899195	1626307	3.01%	1.070%
8	13.280	1691	1699	1716	rBV	14203368	19086914	35.37%	12.563%
9	14.663	1927	1934	1944	rBV2	1574884	2529750	4.69%	1.665%
10	16.157	2180	2188	2203	rBV	18109801	24467210	45.34%	16.104%
11	17.404	2394	2400	2413	rBV	2967684	4190570	7.77%	2.758%
12	19.997	2834	2841	2845	rBV	47025387	53960069	100.00%	35.517%
13	21.544	3099	3104	3111	rBV	4681496	6063202	11.24%	3.991%
14	23.833	3487	3493	3506	rVB	2843035	5334908	9.89%	3.511%


Sum of corrected areas: 151929304

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016510.D
Acq On : 22 Aug 2018 08:35
Operator : SJ/JU
Sample : J4271-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HR-06-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

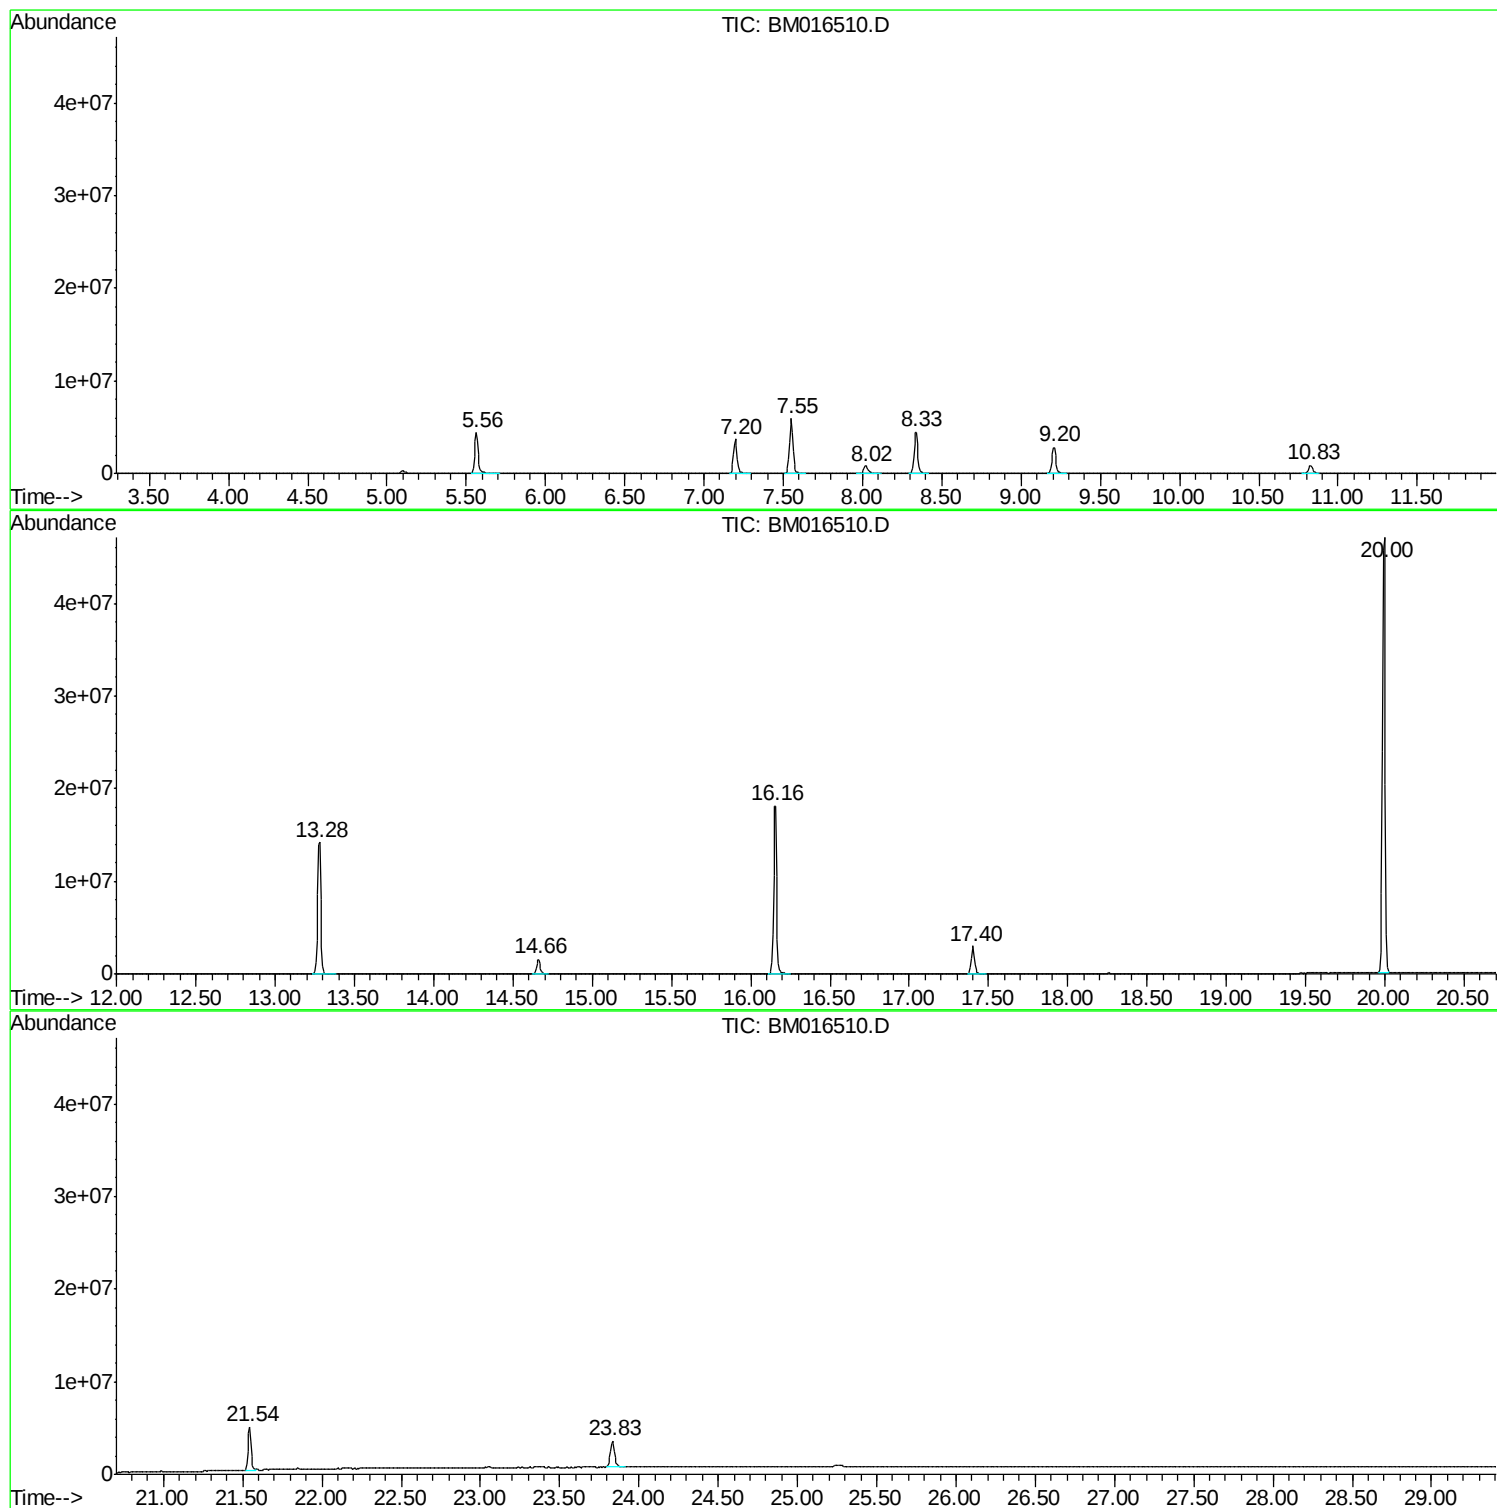

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016510.D
Acq On : 22 Aug 2018 08:35
Operator : SJ/JU
Sample : J4271-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HR-06-082018-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.55	122.38 ng	9005820	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	12

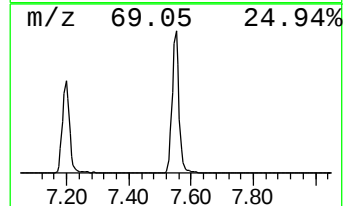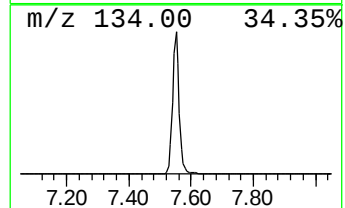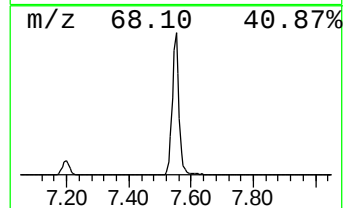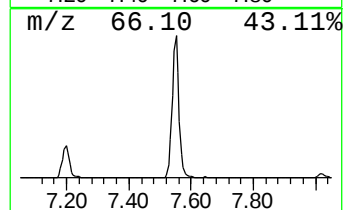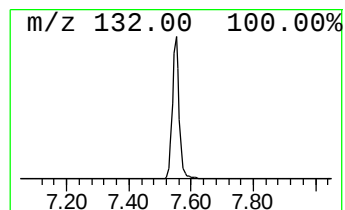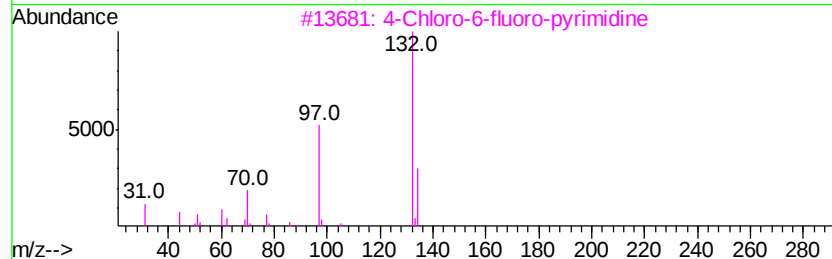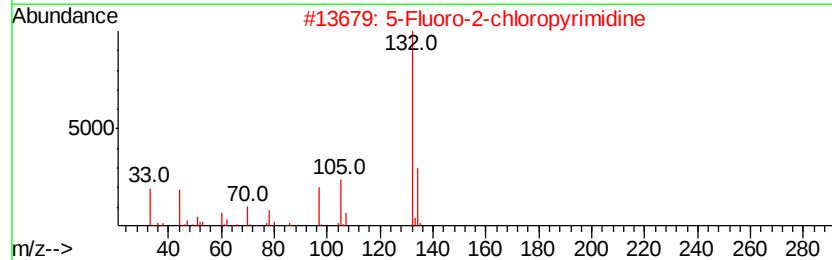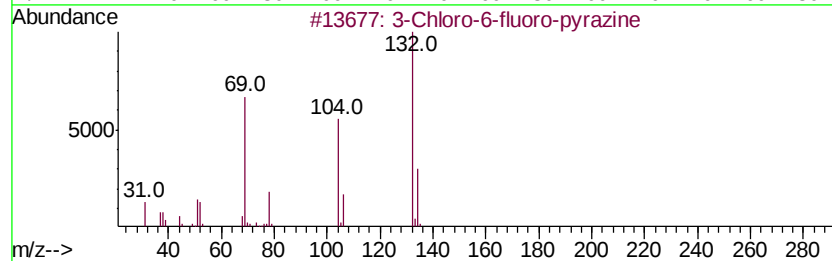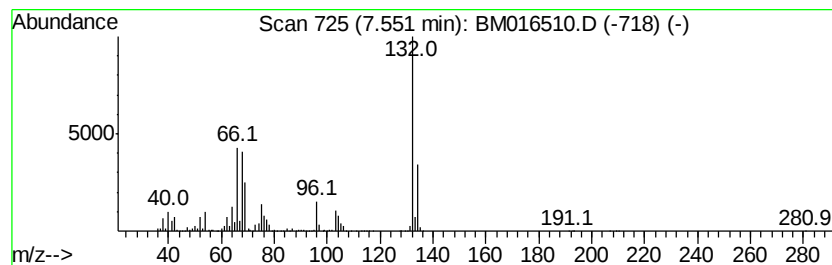

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082118\
Data File : BM016510.D
Acq On : 22 Aug 2018 08:35
Operator : SJ/JU
Sample : J4271-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HR-06-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.55	7.55	122.4	ng	9005820	1	8.02	1471810	20.0