

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
 Data File : BM016513.D
 Acq On : 22 Aug 2018 10:23
 Operator : SJ/JU
 Sample : J4275-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-01-082018-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	382	387	398	rBV	3357706	4895825	11.79%	4.203%
2	7.198	658	665	682	rVB	2728028	4296926	10.35%	3.689%
3	7.551	718	725	744	rBV	4711342	7271884	17.51%	6.243%
4	8.022	800	805	816	rBV	641263	1122684	2.70%	0.964%
5	8.340	852	859	875	rBV	3445679	5522149	13.30%	4.741%
6	9.204	1000	1006	1025	rBV	2307282	3861861	9.30%	3.316%
7	10.828	1275	1282	1294	rBV	677363	1235820	2.98%	1.061%
8	13.280	1692	1699	1712	rBV	10931172	14511047	34.94%	12.459%
9	14.663	1926	1934	1943	rBV2	1170024	1892229	4.56%	1.625%
10	16.157	2181	2188	2205	rBV	14708825	19405632	46.73%	16.661%
11	17.404	2394	2400	2414	rBV	2102501	3136038	7.55%	2.692%
12	19.992	2834	2840	2847	rBV	37906664	41526688	100.00%	35.653%
13	21.545	3099	3104	3111	rBV	3274611	4107521	9.89%	3.527%
14	23.833	3487	3493	3502	rBV	1909769	3687943	8.88%	3.166%


Sum of corrected areas: 116474247

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016513.D
Acq On : 22 Aug 2018 10:23
Operator : SJ/JU
Sample : J4275-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

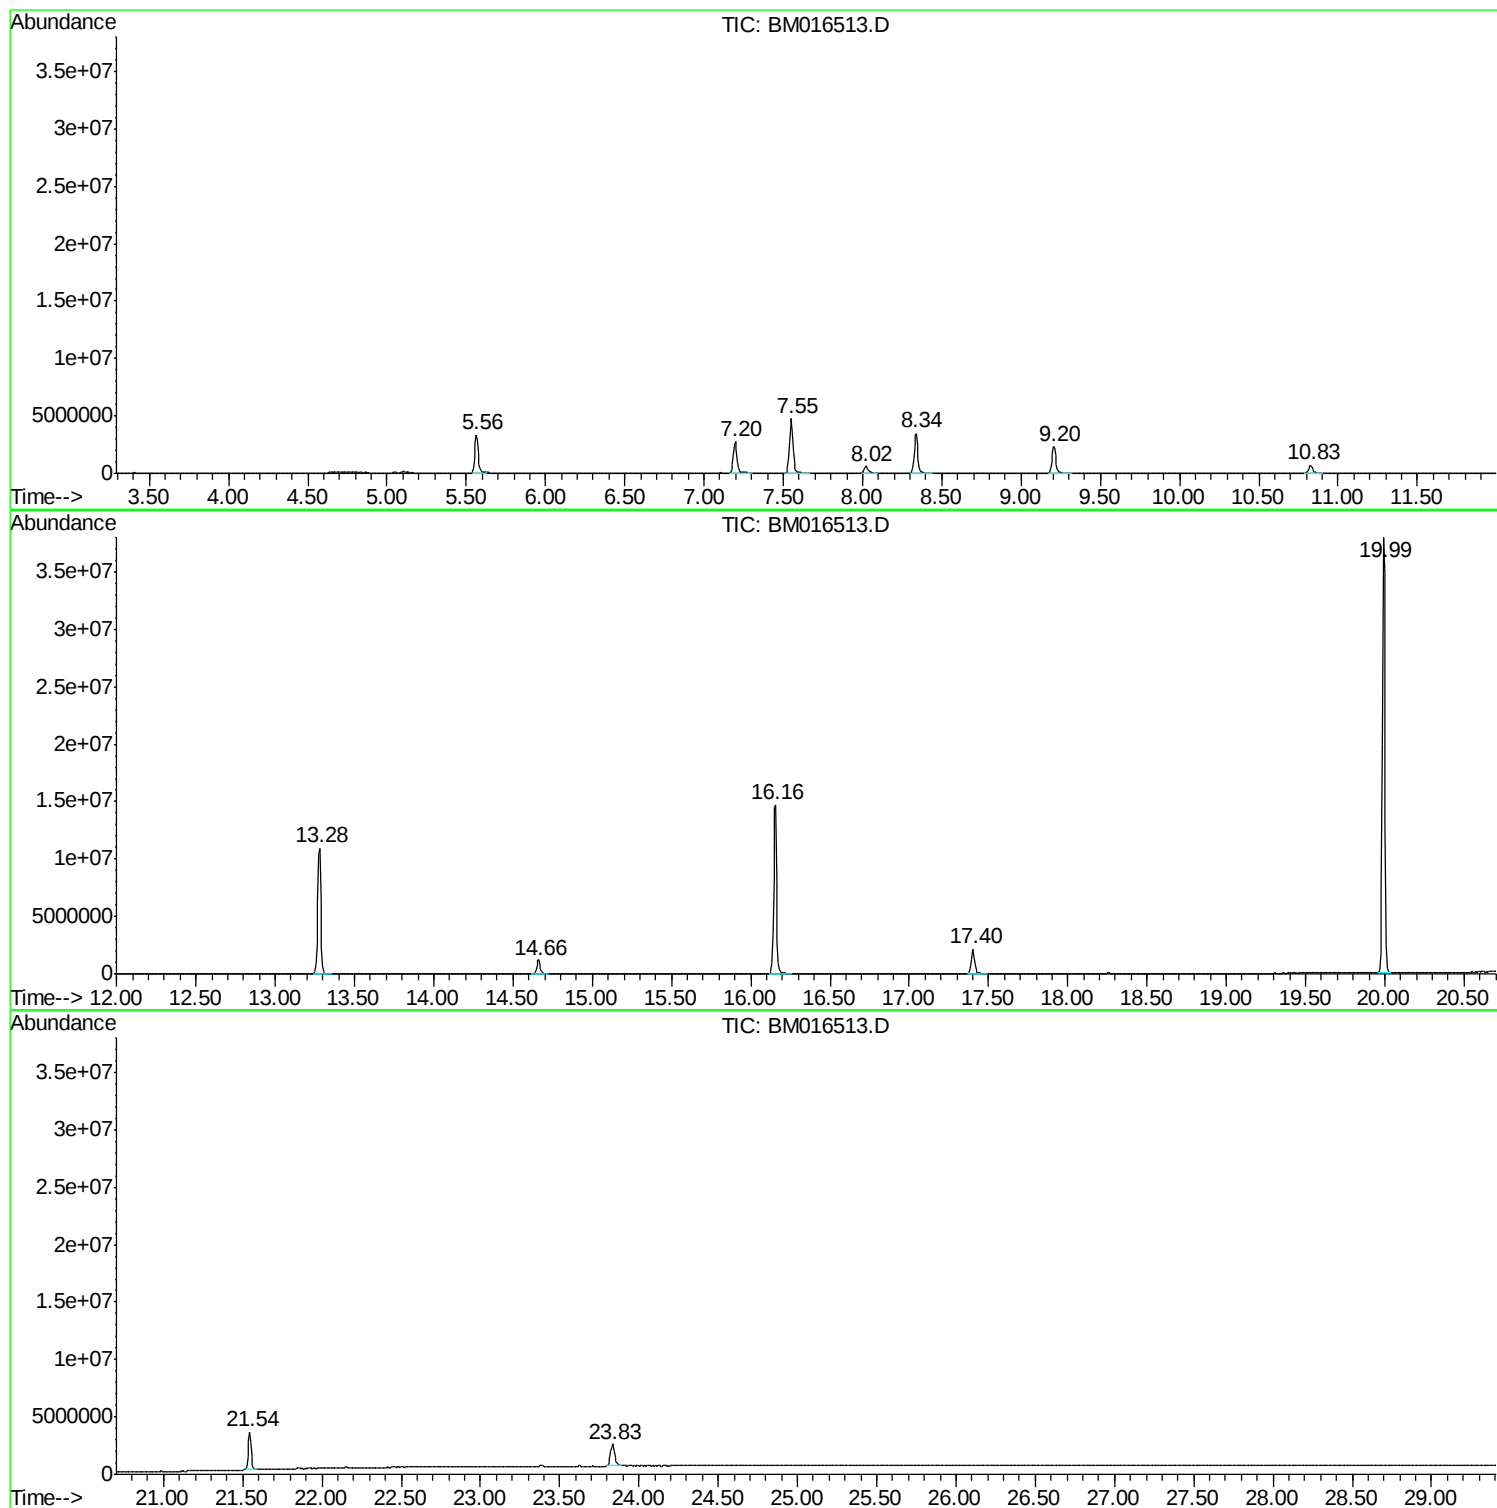

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016513.D
Acq On : 22 Aug 2018 10:23
Operator : SJ/JU
Sample : J4275-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.55	129.55 ng	7271880	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	10

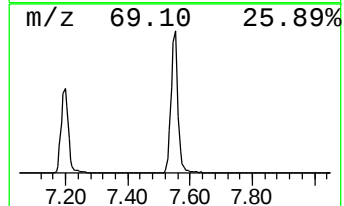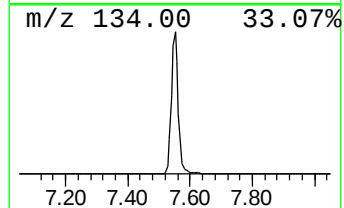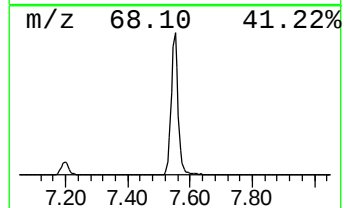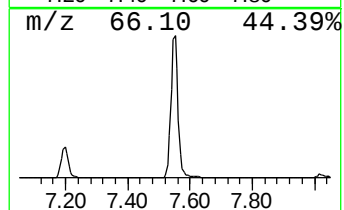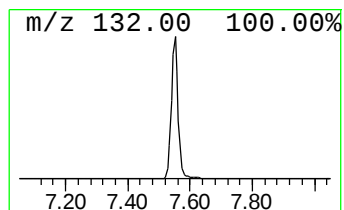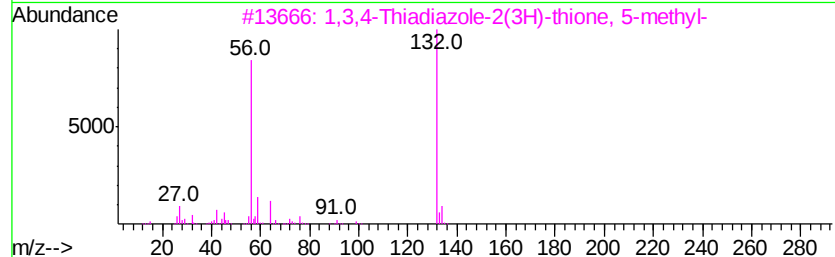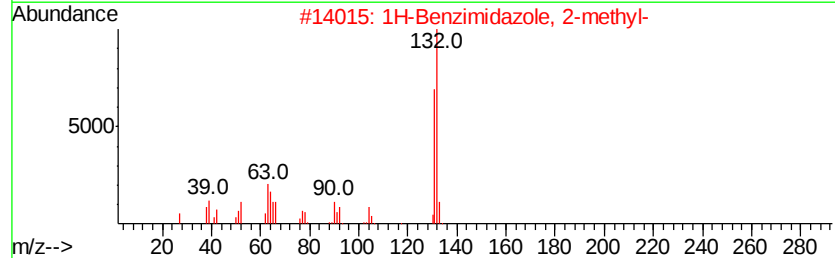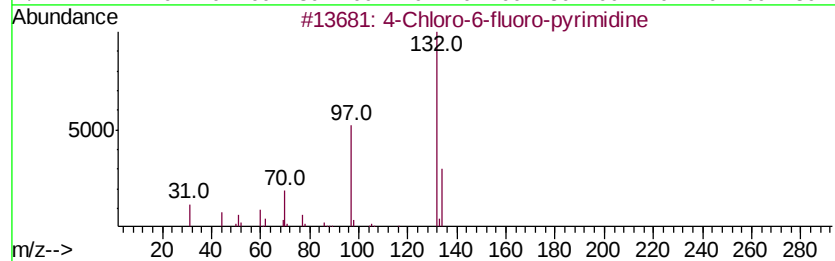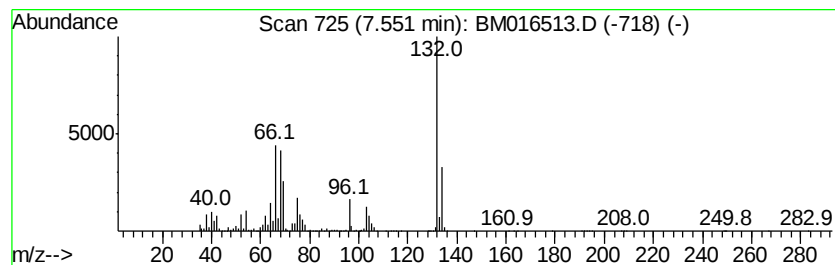

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082118\
Data File : BM016513.D
Acq On : 22 Aug 2018 10:23
Operator : SJ/JU
Sample : J4275-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.55	7.55	129.6	ng	7271880	1	8.02	1122680	20.0