

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
 Data File : BM016514.D
 Acq On : 22 Aug 2018 11:00
 Operator : SJ/JU
 Sample : J4275-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-01-082018-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	381	387	401	rBV	2720564	4078505	13.53%	4.553%
2	7.193	658	664	680	rBV	2414537	3832831	12.72%	4.279%
3	7.546	718	724	740	rBV	3616019	5803162	19.25%	6.479%
4	8.022	799	805	816	rBV	552353	975189	3.24%	1.089%
5	8.334	850	858	870	rBV	2780105	4556213	15.12%	5.087%
6	9.204	998	1006	1018	rBV	1768725	3006485	9.97%	3.357%
7	10.828	1274	1282	1300	rBV	567802	1081295	3.59%	1.207%
8	13.275	1692	1698	1709	rBV	8190489	10983945	36.44%	12.263%
9	14.657	1925	1933	1943	rBV2	942315	1543972	5.12%	1.724%
10	16.151	2181	2187	2206	rBV	10719671	14023762	46.53%	15.657%
11	17.404	2394	2400	2414	rBV2	1571205	2466651	8.18%	2.754%
12	19.992	2834	2840	2851	rBV	29018904	30140250	100.00%	33.650%
13	21.545	3099	3104	3114	rBV	2616441	3627055	12.03%	4.049%
14	23.833	3487	3493	3503	rBV	1744939	3451016	11.45%	3.853%


Sum of corrected areas: 89570331

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016514.D
Acq On : 22 Aug 2018 11:00
Operator : SJ/JU
Sample : J4275-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

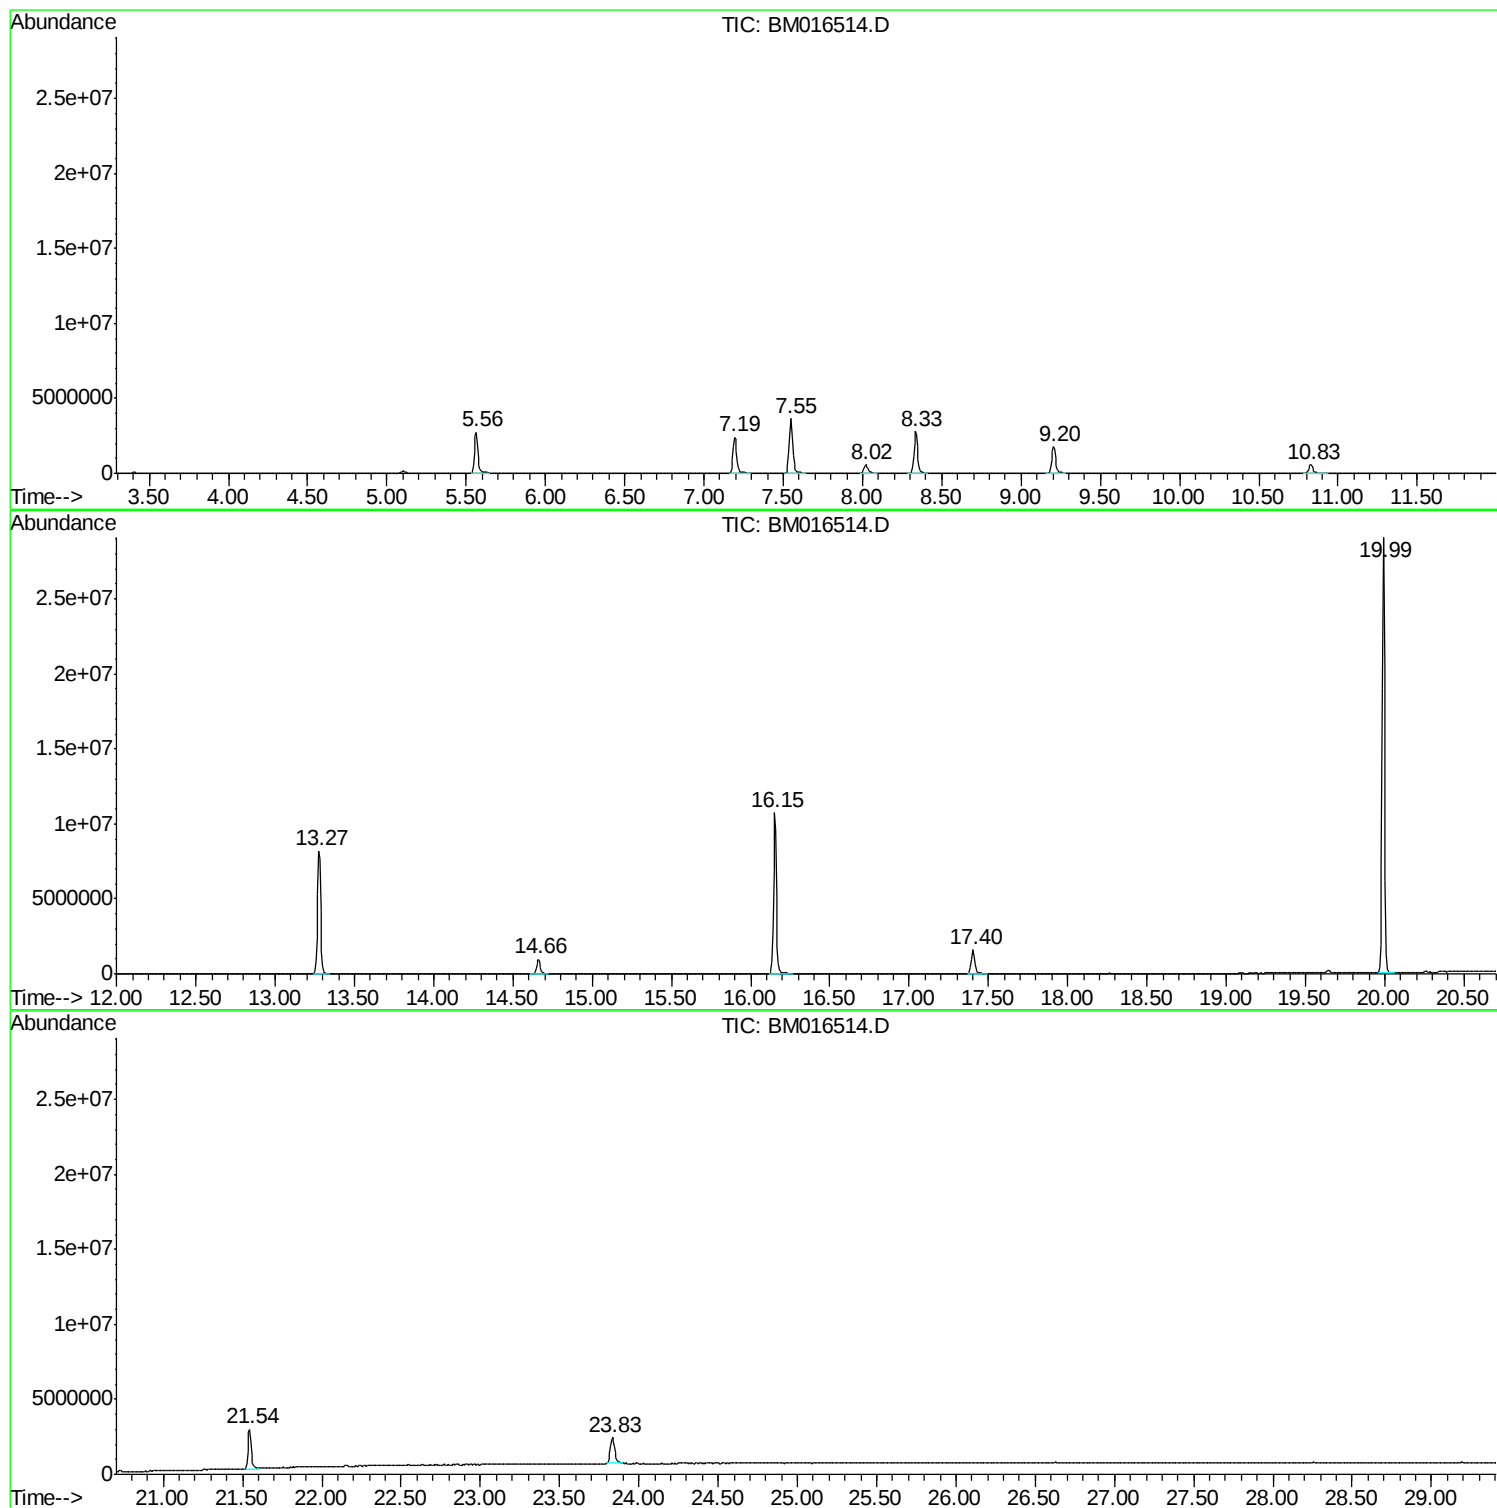

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016514.D
Acq On : 22 Aug 2018 11:00
Operator : SJ/JU
Sample : J4275-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-D










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.55	119.02 ng	5803160	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	10
5		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10

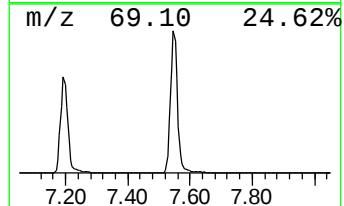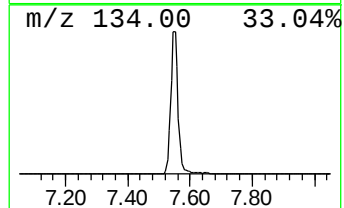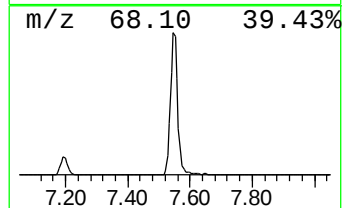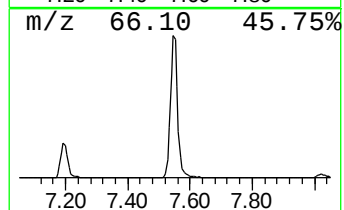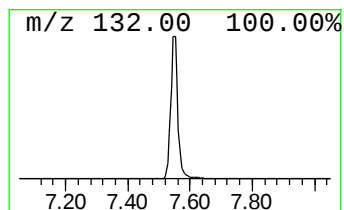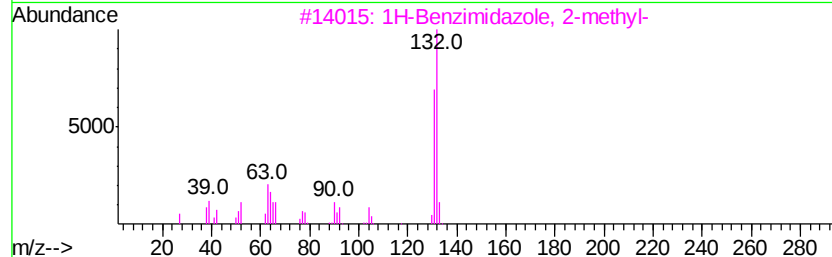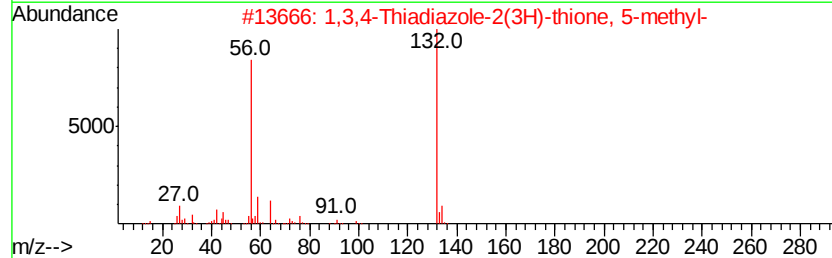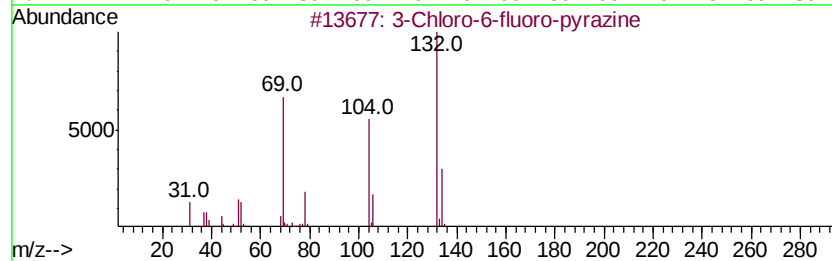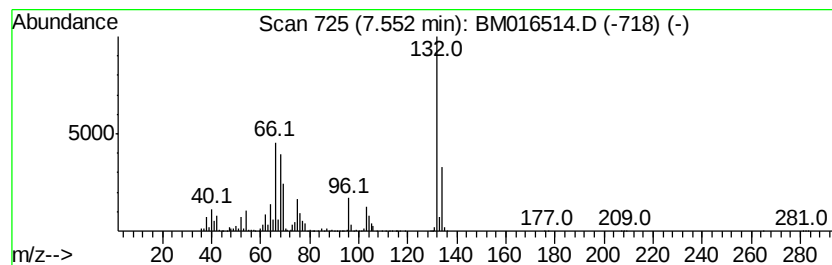

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082118\
Data File : BM016514.D
Acq On : 22 Aug 2018 11:00
Operator : SJ/JU
Sample : J4275-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.55	7.55	119.0	ng	5803160	1	8.02	975189	20.0