

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
 Data File : BM016515.D
 Acq On : 22 Aug 2018 11:36
 Operator : SJ/JU
 Sample : J4275-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-01-082018-E

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	381	387	406	rBV	2560343	3943488	13.66%	4.451%
2	7.193	658	664	678	rBV	2144579	3447355	11.94%	3.891%
3	7.546	718	724	740	rBV	3651115	5784599	20.04%	6.529%
4	8.022	799	805	820	rBV	593143	1058632	3.67%	1.195%
5	8.334	852	858	871	rBV	2872518	4625027	16.02%	5.220%
6	9.204	999	1006	1026	rBV	1829283	3125139	10.83%	3.527%
7	10.828	1275	1282	1289	rBV	636598	1157799	4.01%	1.307%
8	13.275	1692	1698	1715	rBV	7984676	11139241	38.59%	12.572%
9	14.663	1927	1934	1942	rBV2	1025560	1682373	5.83%	1.899%
10	16.151	2181	2187	2205	rBV	10282336	13704598	47.48%	15.468%
11	17.404	2394	2400	2415	rBV	1787797	2700164	9.35%	3.048%
12	19.992	2834	2840	2850	rBV	27515710	28864361	100.00%	32.578%
13	21.545	3099	3104	3115	rBV	2800999	3753035	13.00%	4.236%
14	23.833	3487	3493	3507	rBV	1866468	3616252	12.53%	4.081%


Sum of corrected areas: 88602063

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016515.D
Acq On : 22 Aug 2018 11:36
Operator : SJ/JU
Sample : J4275-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

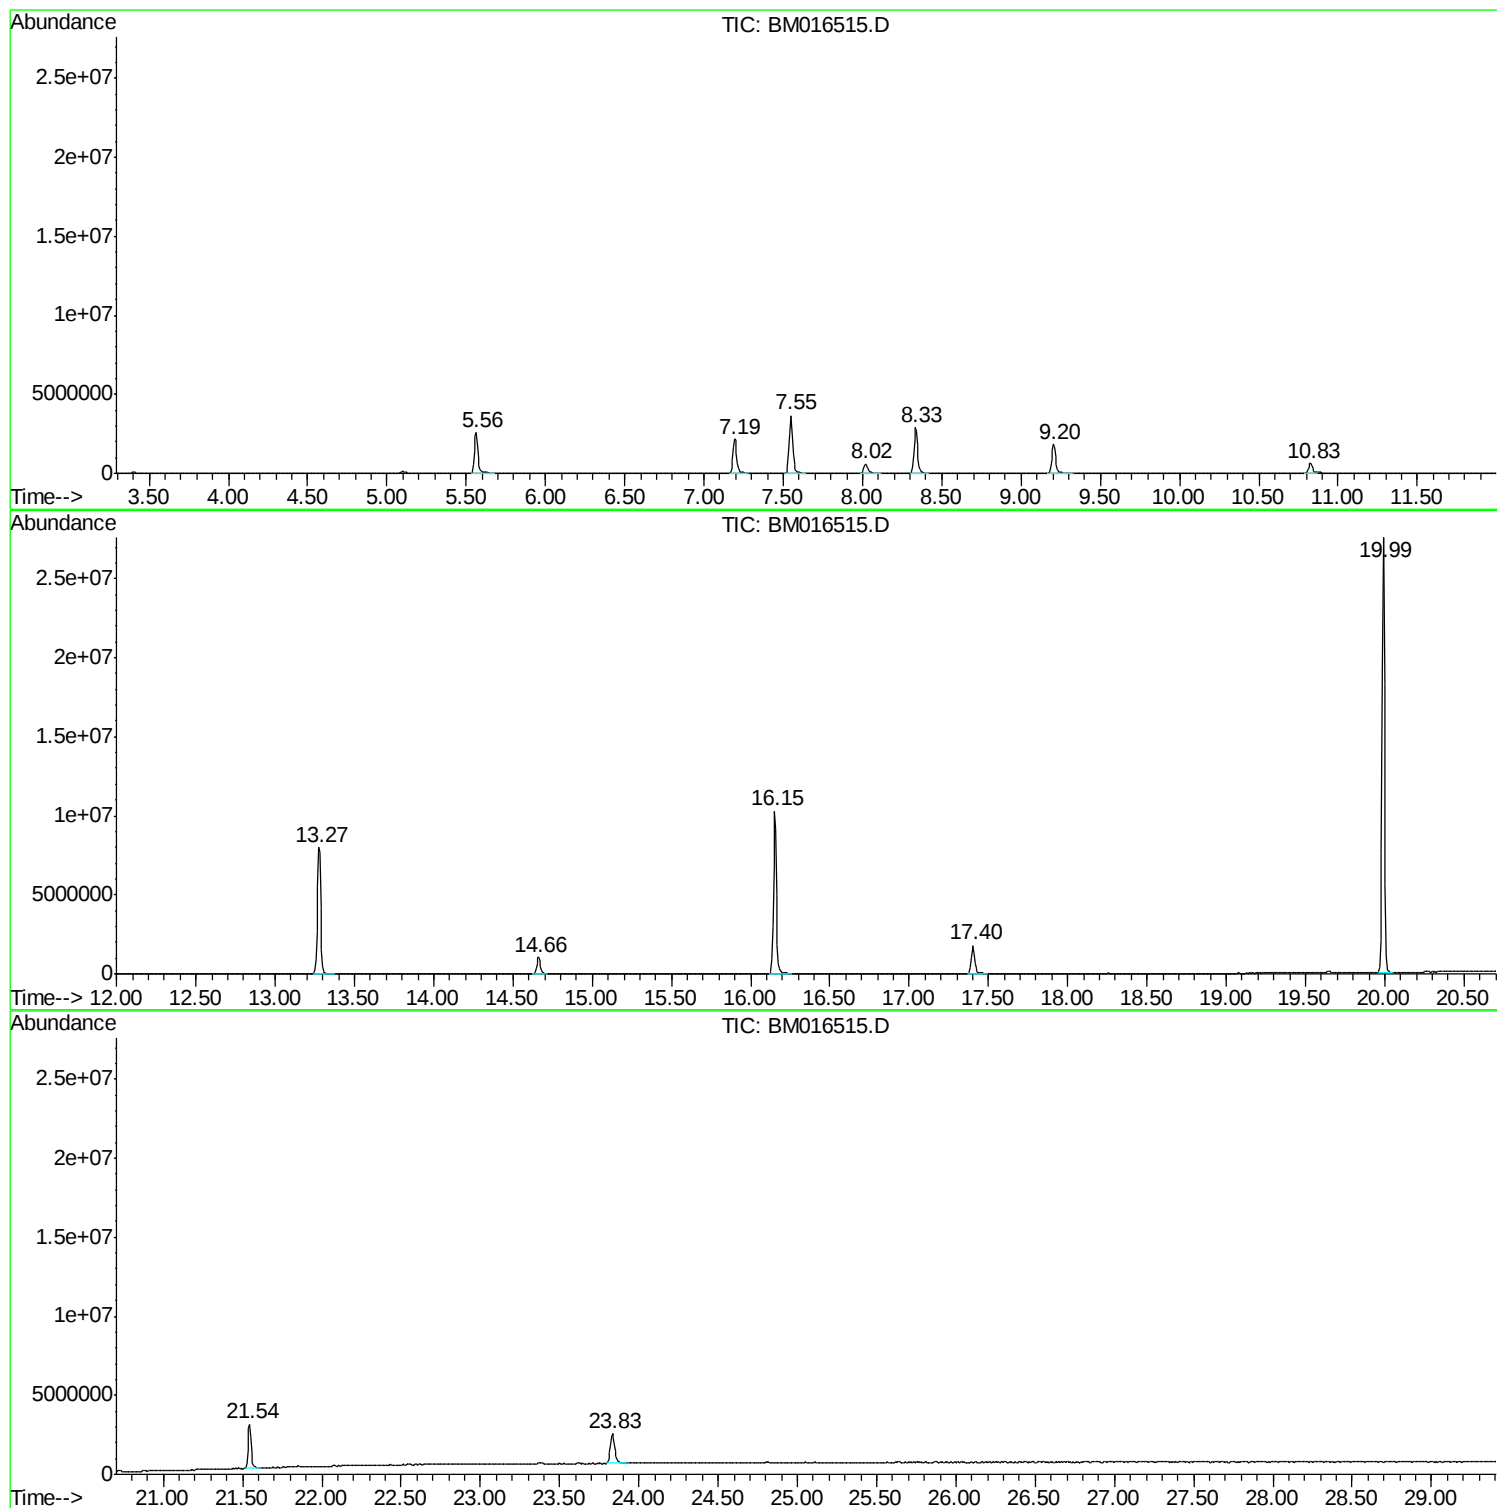

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082118\
Data File : BM016515.D
Acq On : 22 Aug 2018 11:36
Operator : SJ/JU
Sample : J4275-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-E










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.55 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.55	109.28 ng	5784600	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	10
2		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

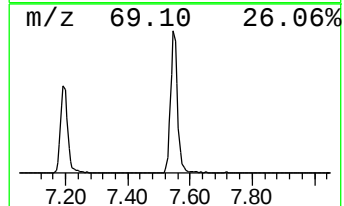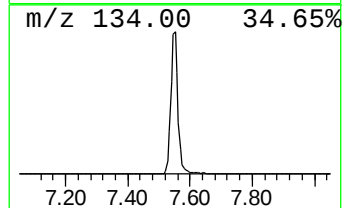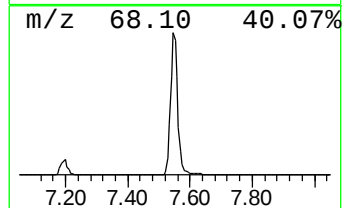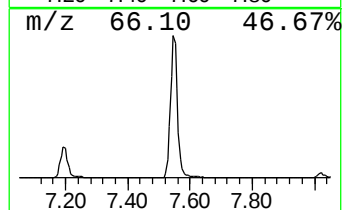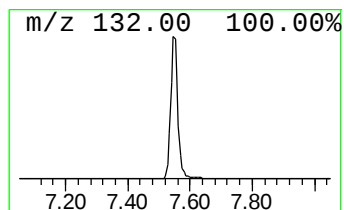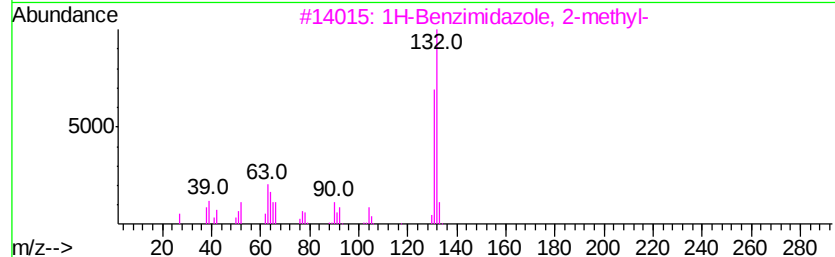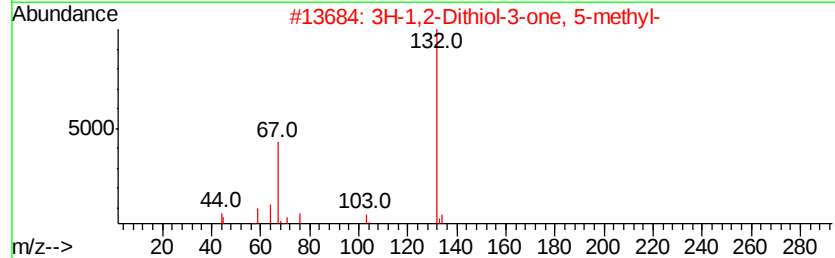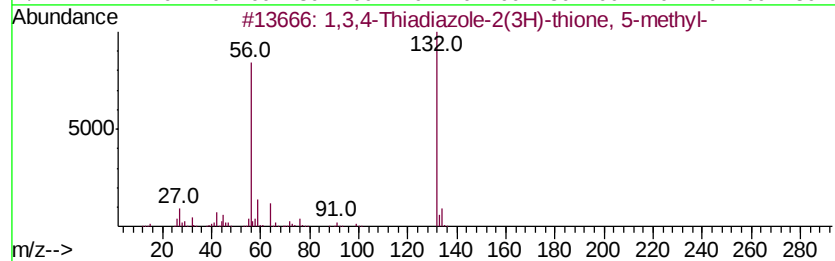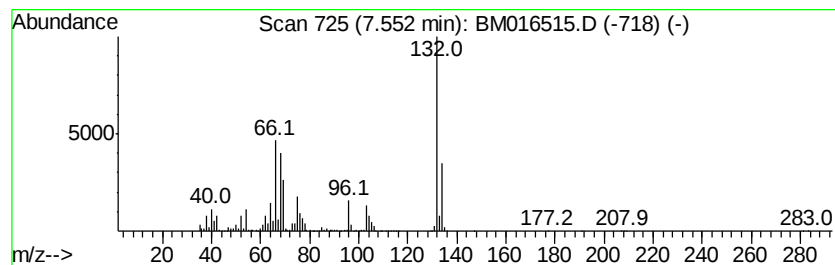

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082118\
Data File : BM016515.D
Acq On : 22 Aug 2018 11:36
Operator : SJ/JU
Sample : J4275-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-01-082018-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.55	7.55	109.3	ng	5784600	1	8.02	1058630	20.0