


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082118\
 Data File : BM016479.D
 Acq On : 21 Aug 2018 10:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 21 16:31:22 2018

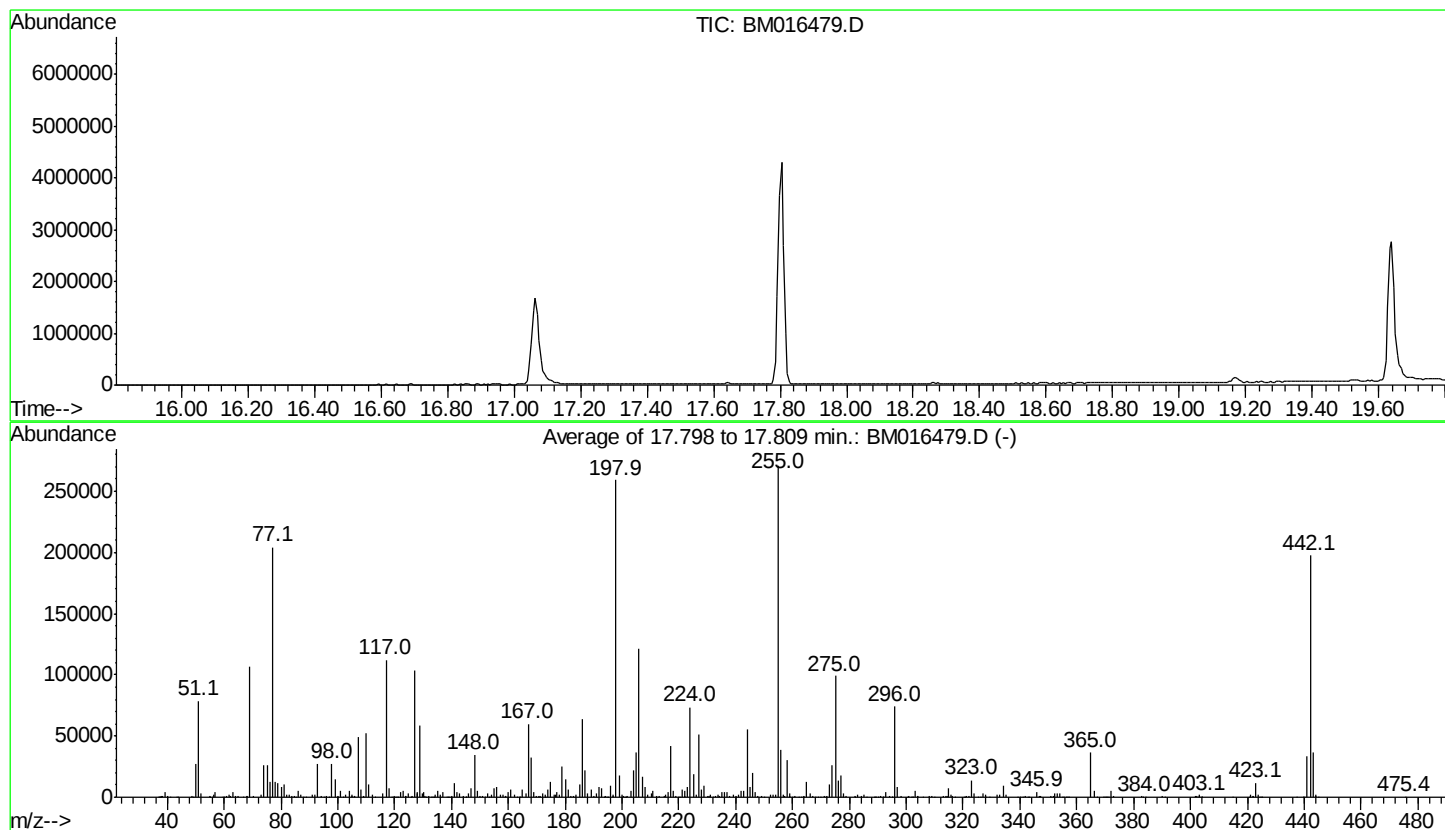

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	78538	PASS
68	69	0.00	2	1.3	1420	PASS
69	198	0.00	100	41.3	106893	PASS
70	69	0.00	2	0.9	942	PASS
127	198	10	80	40.1	103928	PASS
197	198	0.00	2	0.7	1742	PASS
198	198	100	100	100.0	258965	PASS
199	198	5	9	7.1	18317	PASS
275	198	10	60	38.3	99061	PASS
365	198	1	100	14.0	36162	PASS
441	198	0.01	100	12.8	33218	PASS
442	198	50	100	76.2	197397	PASS
443	442	15	24	18.6	36661	PASS