


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082118\
 Data File : BM016489.D
 Acq On : 21 Aug 2018 18:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 21 16:31:22 2018

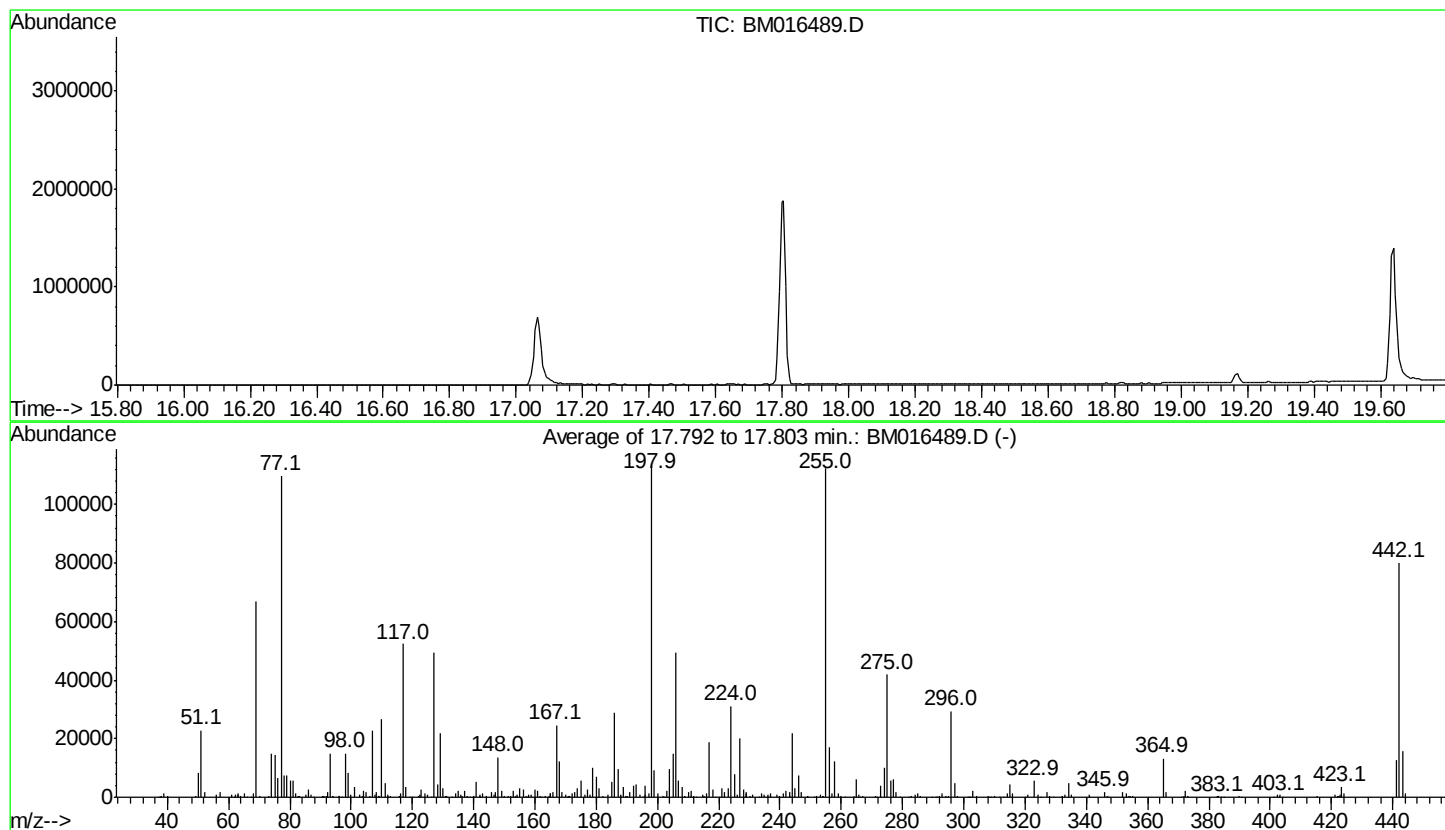

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	22816	PASS
68	69	0.00	2	1.7	1113	PASS
69	198	0.00	100	58.9	66722	PASS
70	69	0.00	2	0.4	251	PASS
127	198	10	80	43.7	49442	PASS
197	198	0.00	2	1.2	1406	PASS
198	198	100	100	100.0	113253	PASS
199	198	5	9	7.9	9000	PASS
275	198	10	60	37.0	41949	PASS
365	198	1	100	11.8	13312	PASS
441	198	0.01	100	11.1	12596	PASS
442	198	50	100	70.8	80189	PASS
443	442	15	24	19.9	15941	PASS