


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082118\
 Data File : BM016508.D
 Acq On : 22 Aug 2018 07:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 21 16:31:22 2018

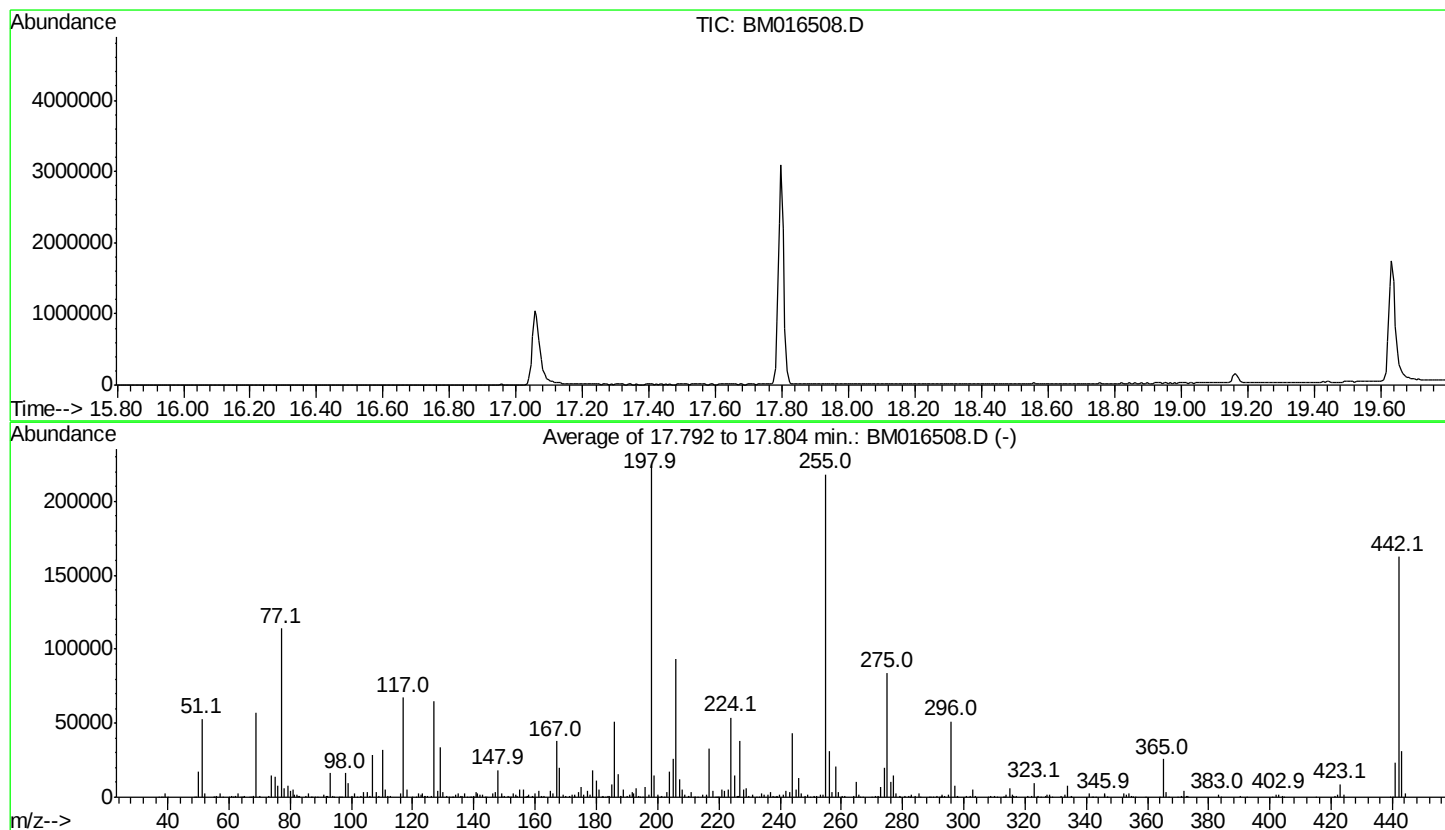

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	52776	PASS
68	69	0.00	2	1.9	1115	PASS
69	198	0.00	100	25.6	57378	PASS
70	69	0.00	2	0.9	505	PASS
127	198	10	80	29.1	65141	PASS
197	198	0.00	2	0.9	2084	PASS
198	198	100	100	100.0	224021	PASS
199	198	5	9	6.7	15089	PASS
275	198	10	60	37.6	84173	PASS
365	198	1	100	11.5	25770	PASS
441	198	0.01	100	10.3	22992	PASS
442	198	50	100	72.5	162458	PASS
443	442	15	24	19.2	31136	PASS