
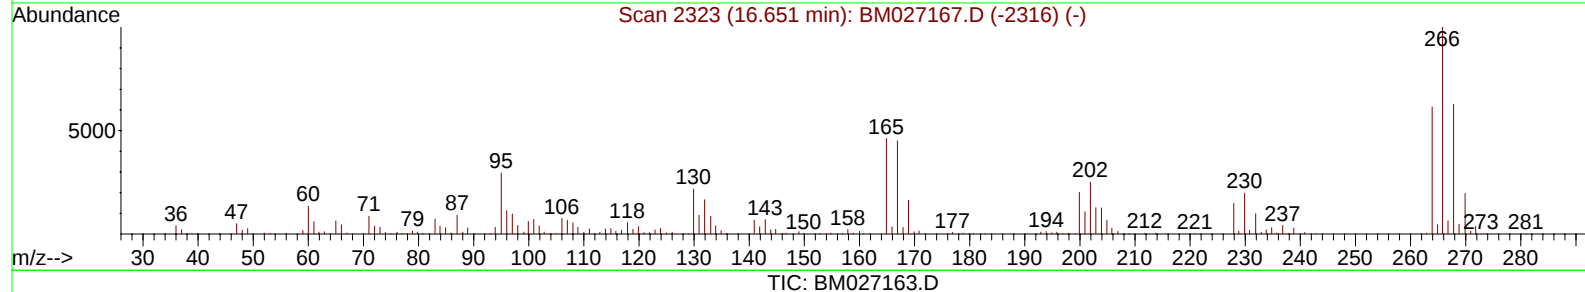
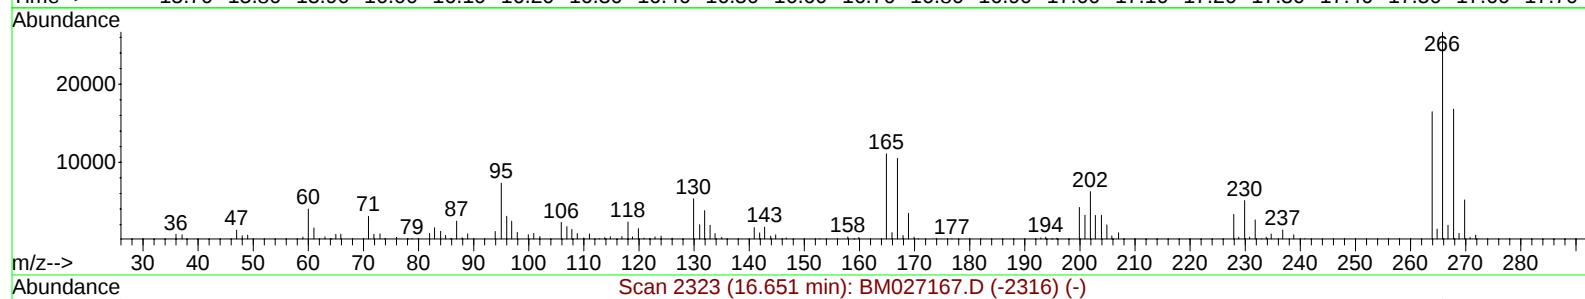


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082120\
Data File : BM027163.D
Acq On : 21 Aug 2020 10:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:34:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 21 15:18:25 2020
Response via : Initial Calibration

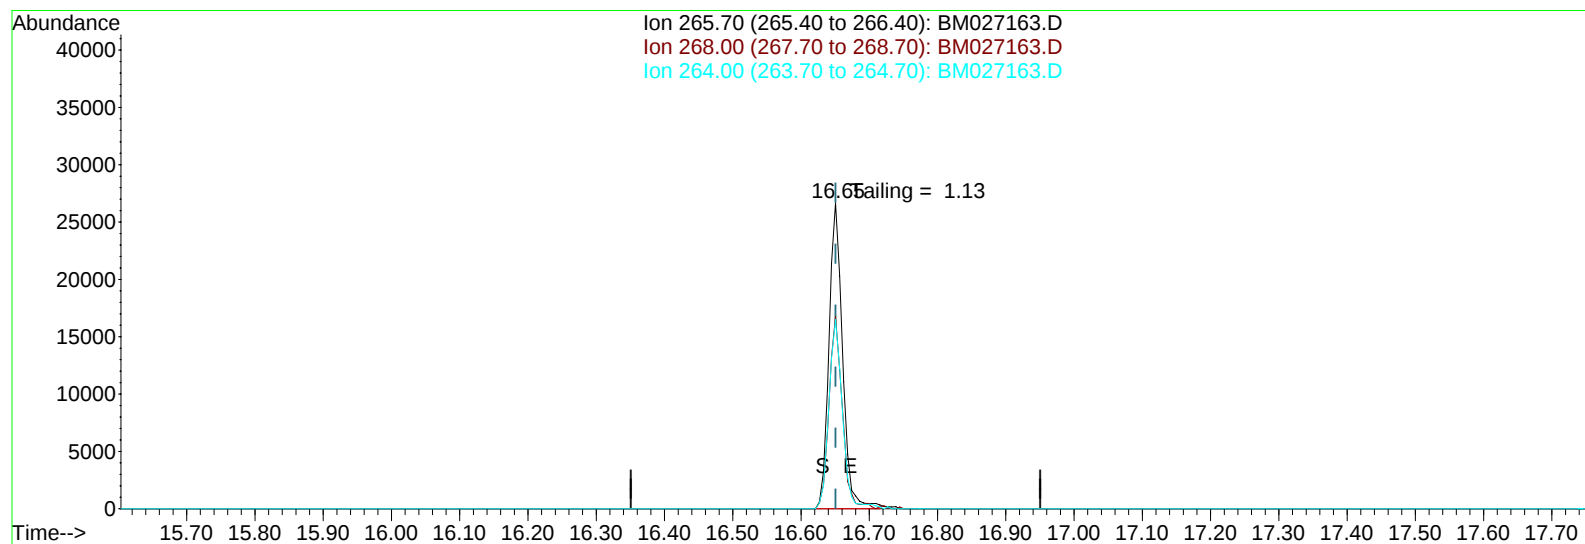

(70) Pentachlorophenol (C)




16.651min (-0.000) 0.00ng

response 36997

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	62.98
264.00	61.40	61.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082120\
 Data File : BM027163.D
 Acq On : 21 Aug 2020 10:08
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:34:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 21 15:18:25 2020
 Response via : Initial Calibration

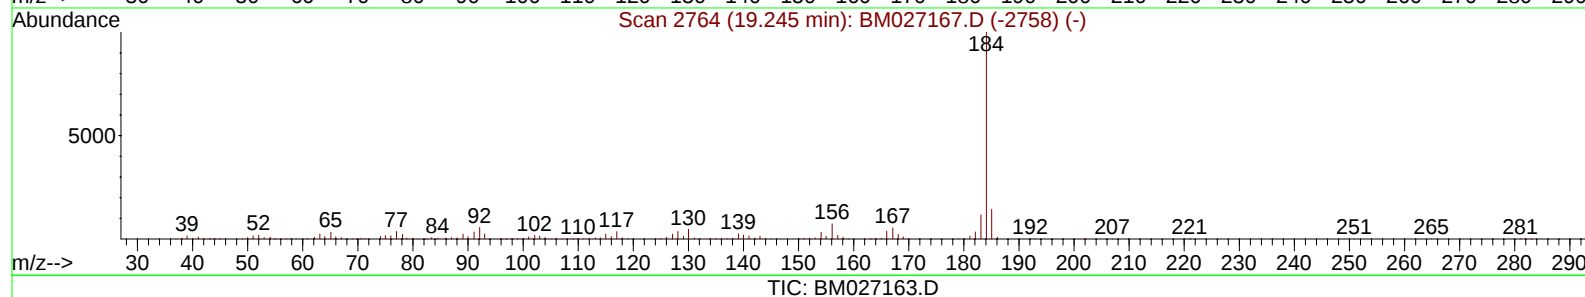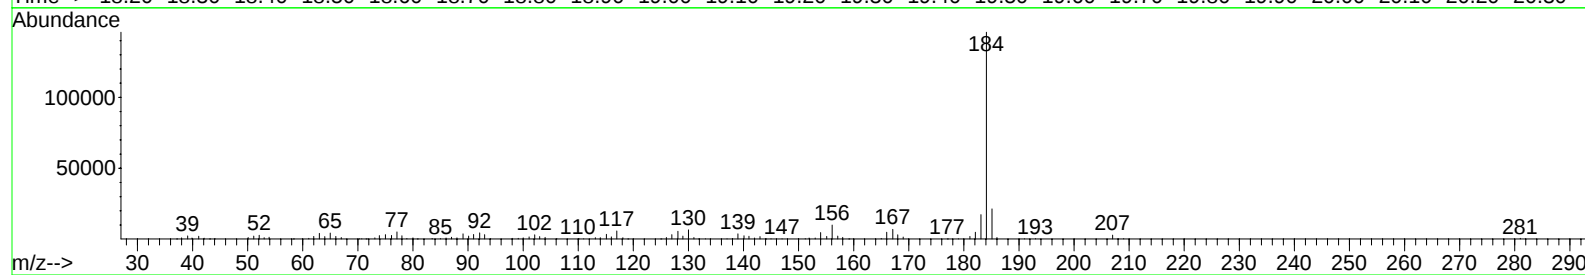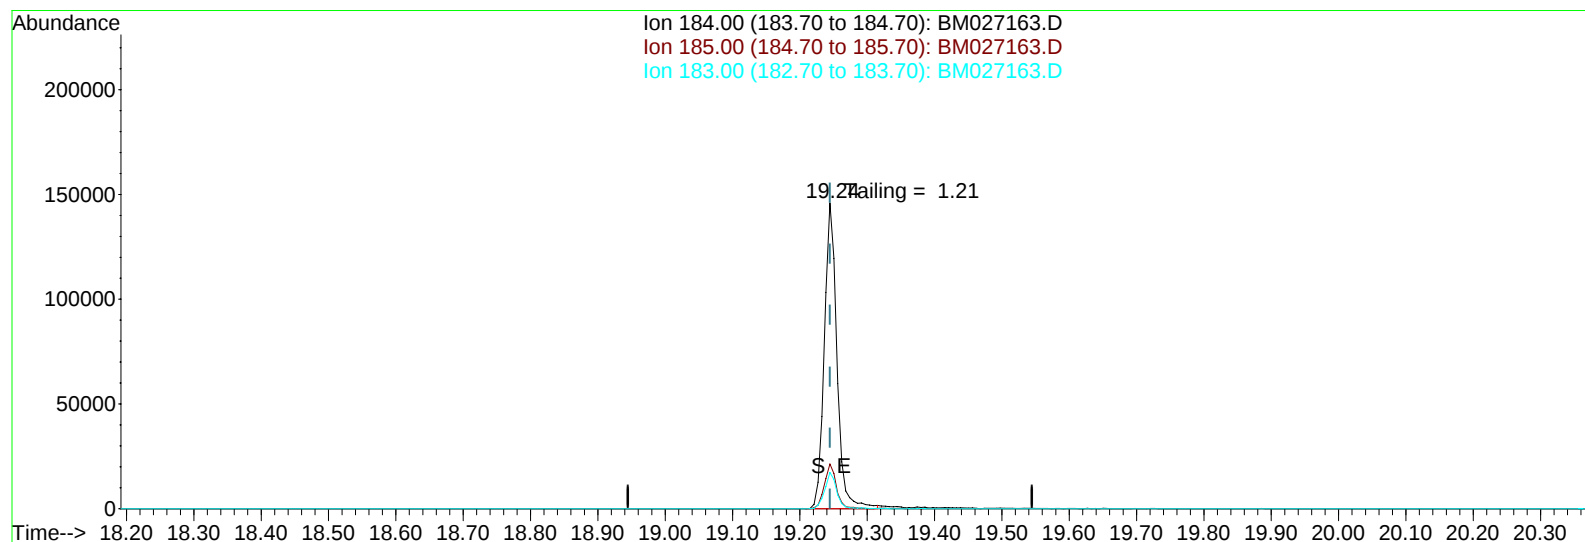

(77) Benzidine

19.245min (-0.000) 0.00ng

response 193089

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.64
183.00	11.70	11.89
0.00	0.00	0.00