
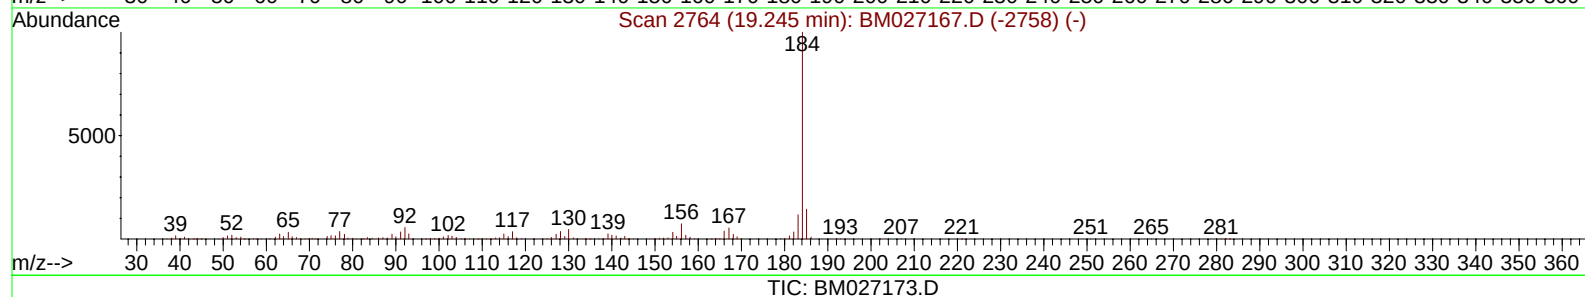
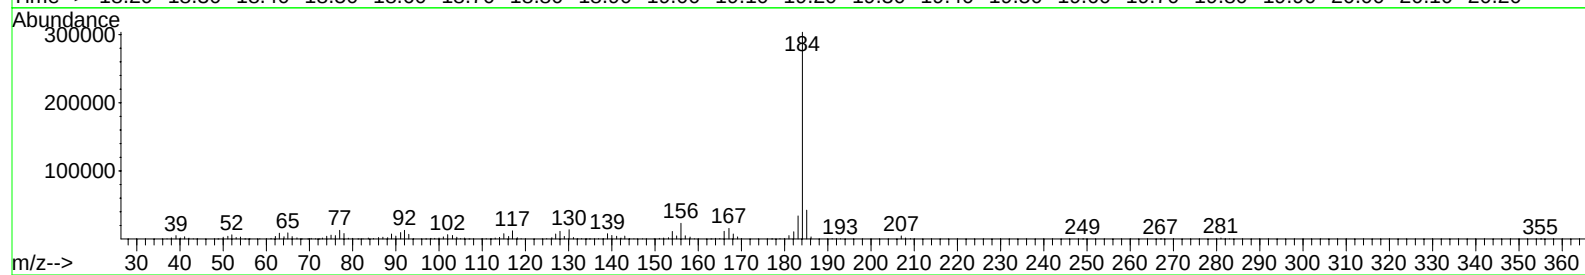


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082120\
 Data File : BM027173.D
 Acq On : 21 Aug 2020 17:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:36:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 21 15:18:25 2020
 Response via : Initial Calibration

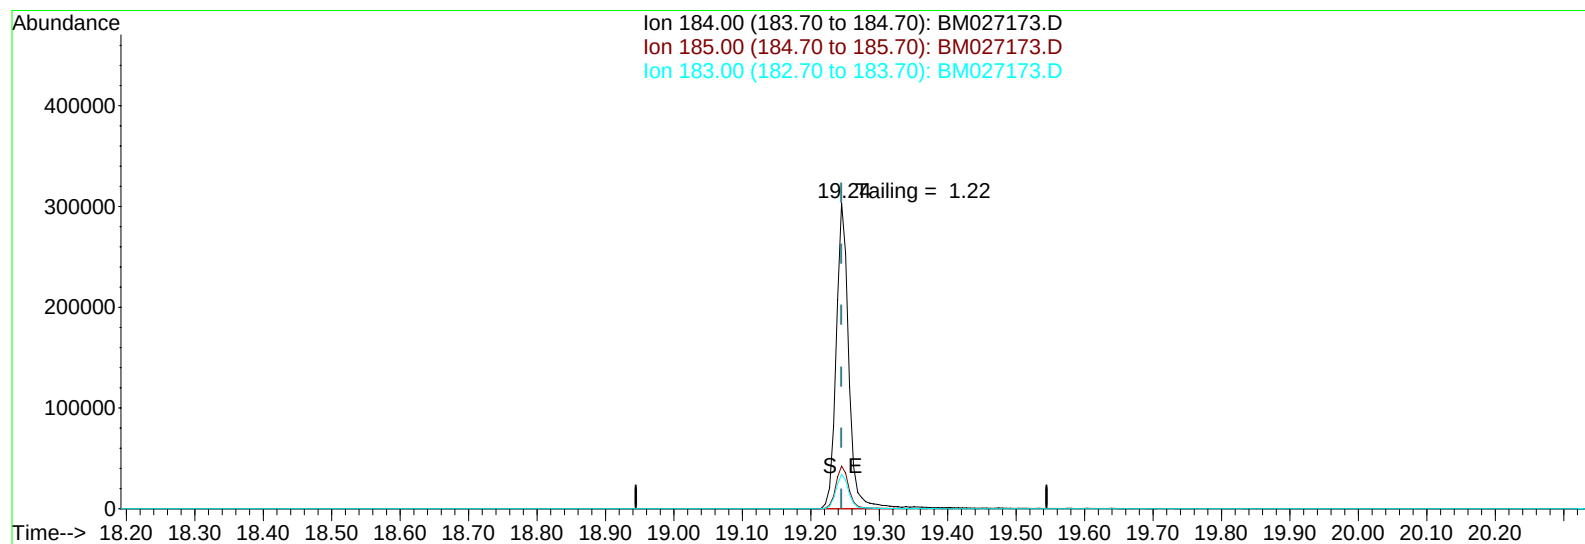

(77) Benzidine




19.245min (+0.000) 0.00ng

response 387530

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.95
183.00	11.70	11.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082120\
Data File : BM027173.D
Acq On : 21 Aug 2020 17:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:36:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 21 15:18:25 2020
Response via : Initial Calibration

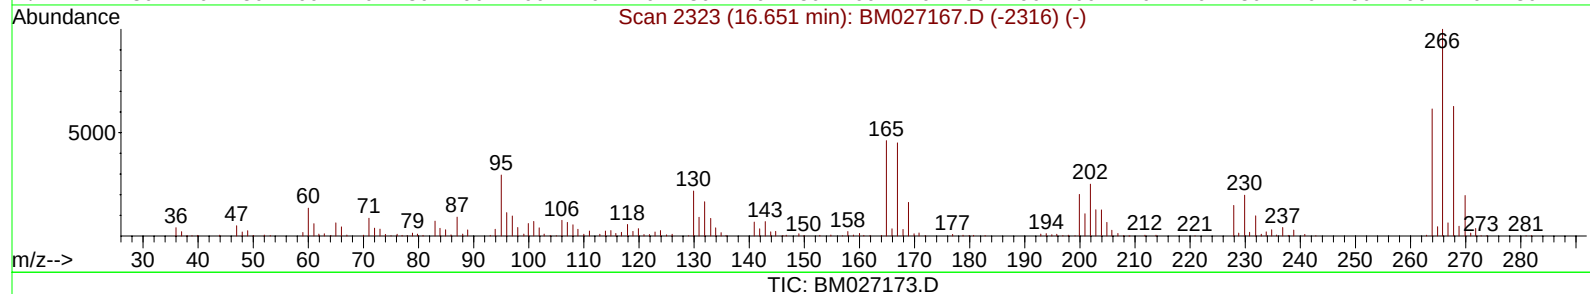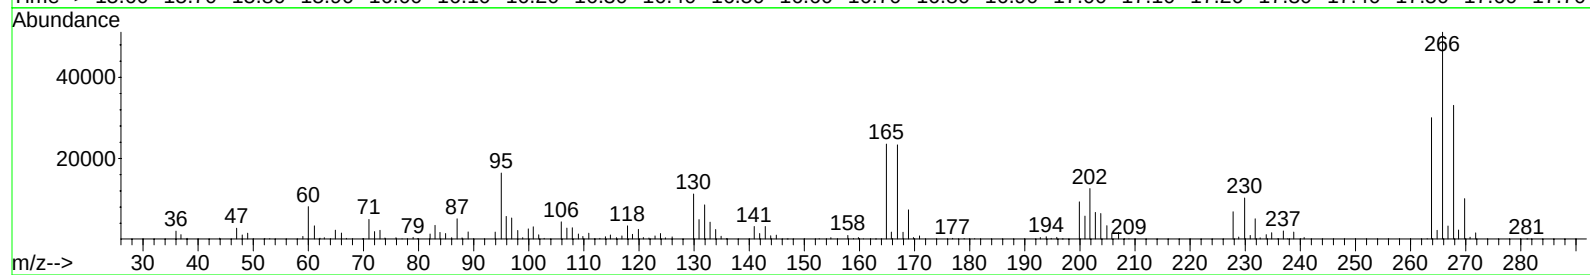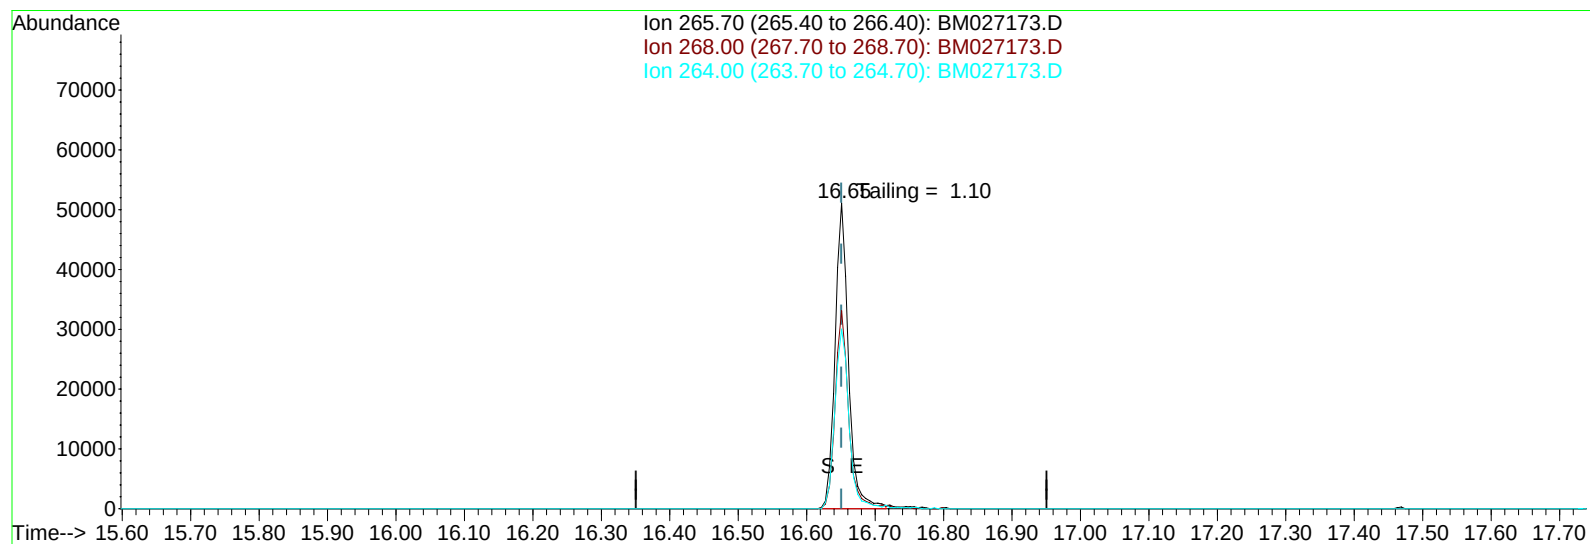

(70) Pentachlorophenol (C)

16.651min (+0.000) 0.00ng

response 70370

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	69.36
264.00	61.40	58.76
0.00	0.00	0.00