


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082120\
 Data File : BM027163.D
 Acq On : 21 Aug 2020 10:08
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:18:39 2020

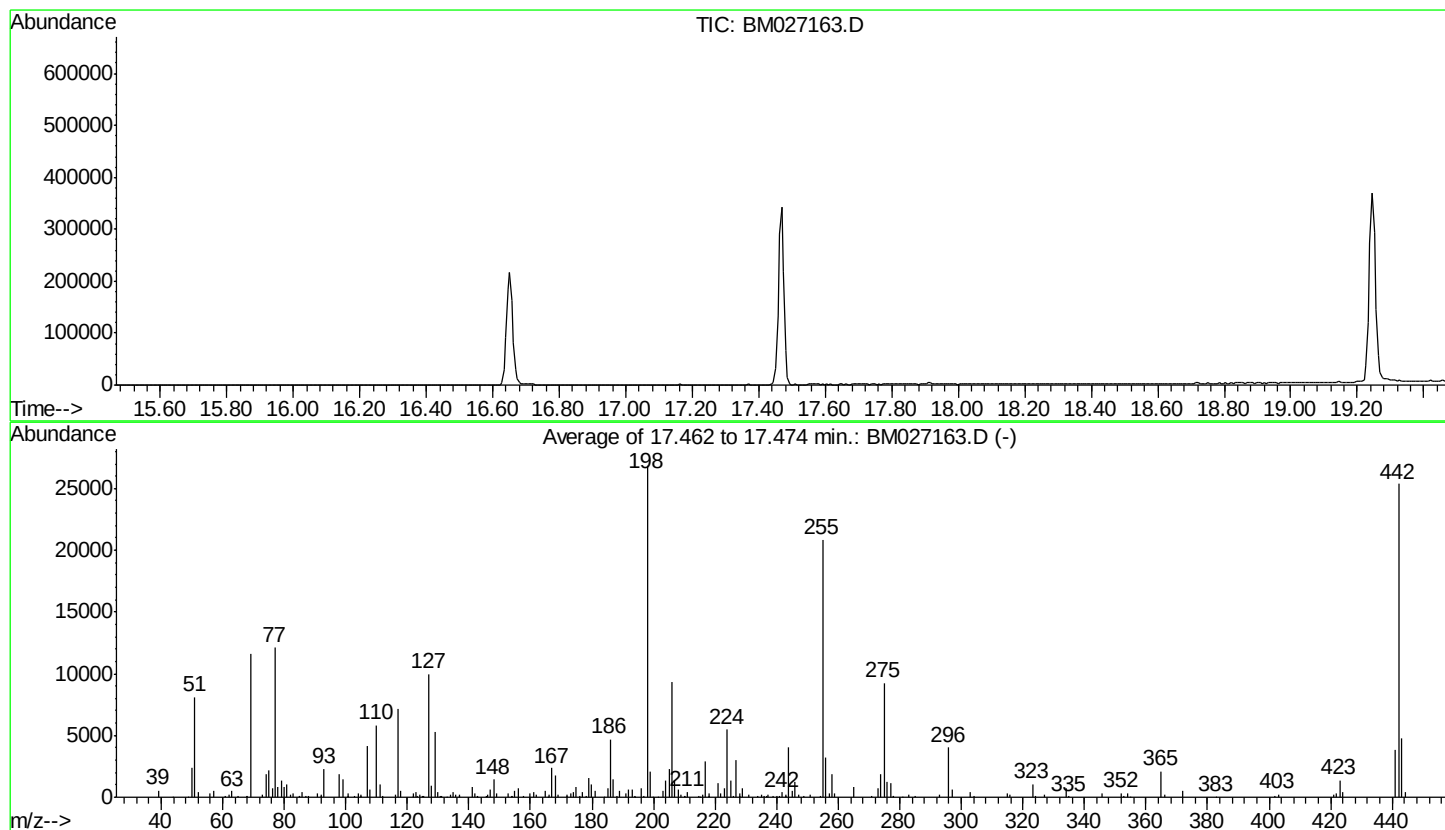

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	8122	PASS
68	69	0.00	2	1.3	154	PASS
69	198	0.00	100	43.4	11662	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.1	9954	PASS
197	198	0.00	2	0.2	58	PASS
198	198	100	100	100.0	26850	PASS
199	198	5	9	7.6	2052	PASS
275	198	10	60	34.4	9230	PASS
365	198	1	100	7.8	2087	PASS
441	198	0.01	100	14.1	3797	PASS
442	198	50	100	94.5	25368	PASS
443	442	15	24	18.9	4803	PASS