


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082120\
 Data File : BM027173.D
 Acq On : 21 Aug 2020 17:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:18:39 2020

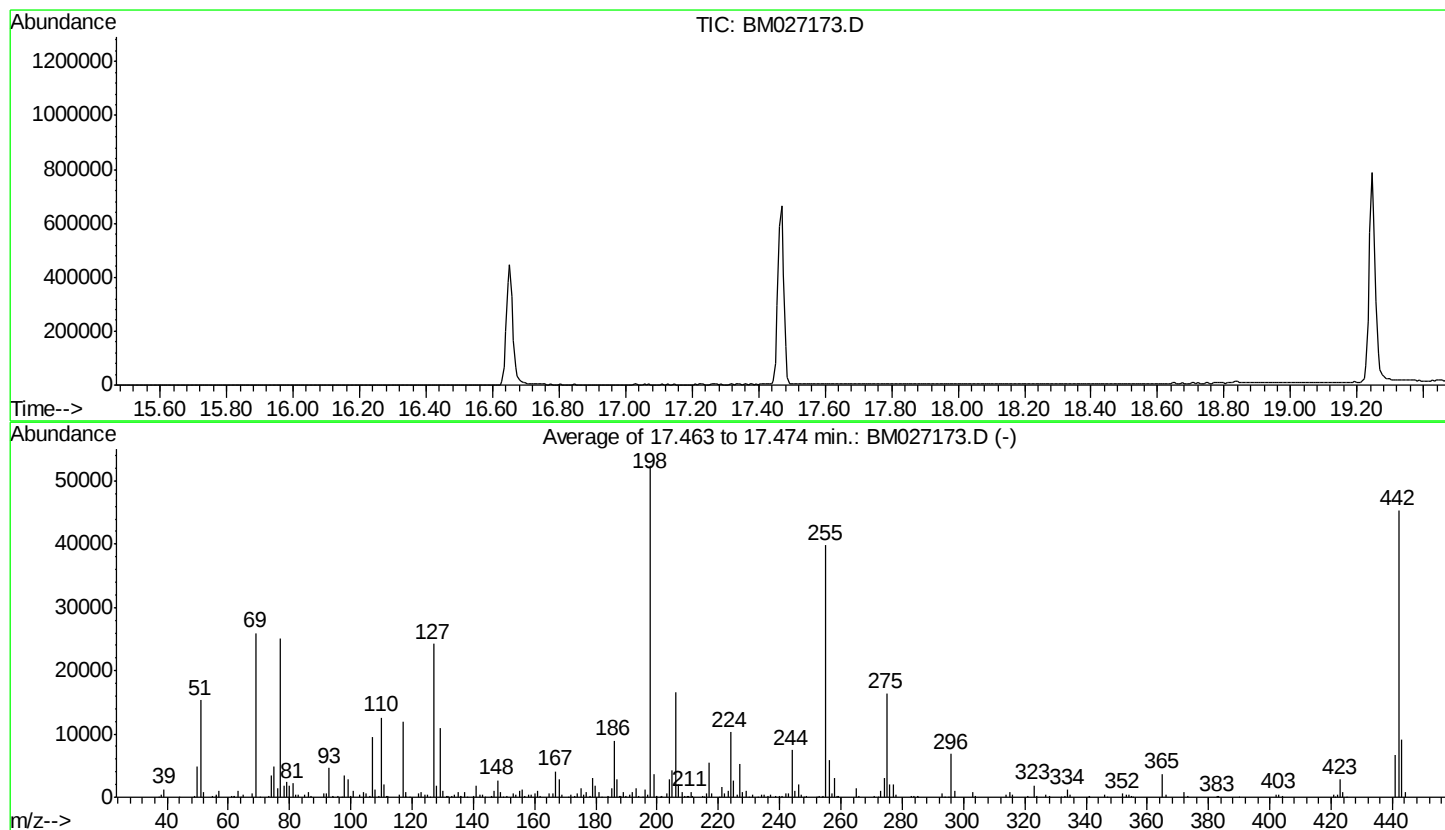

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	15301	PASS
68	69	0.00	2	2.0	514	PASS
69	198	0.00	100	49.5	25926	PASS
70	69	0.00	2	0.3	73	PASS
127	198	10	80	46.3	24266	PASS
197	198	0.00	2	0.7	391	PASS
198	198	100	100	100.0	52424	PASS
199	198	5	9	7.0	3669	PASS
275	198	10	60	31.3	16386	PASS
365	198	1	100	7.0	3647	PASS
441	198	0.01	100	12.8	6724	PASS
442	198	50	100	86.3	45264	PASS
443	442	15	24	20.0	9069	PASS