
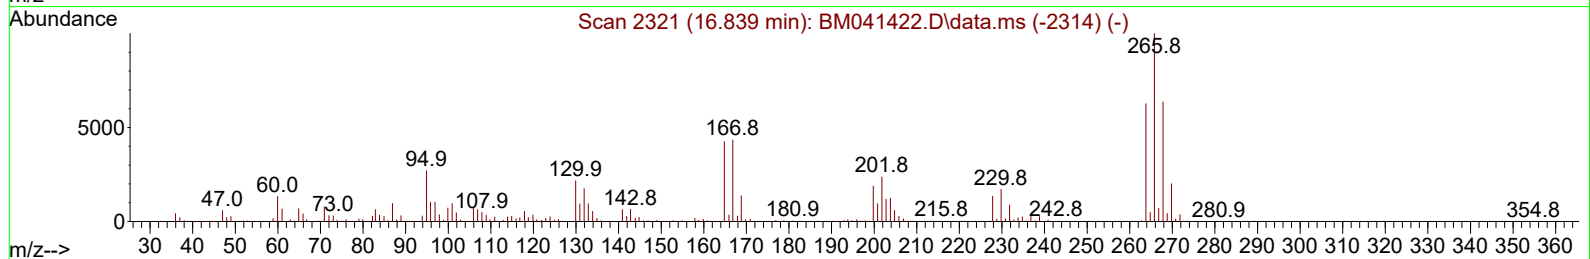
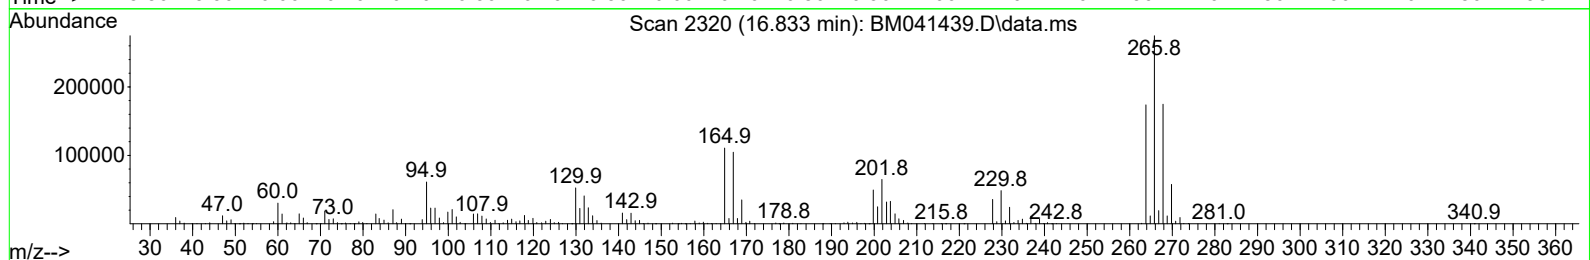


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082123\
Data File : BM041439.D
Acq On : 21 Aug 2023 09:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 04:04:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 03:32:15 2023
Response via : Initial Calibration

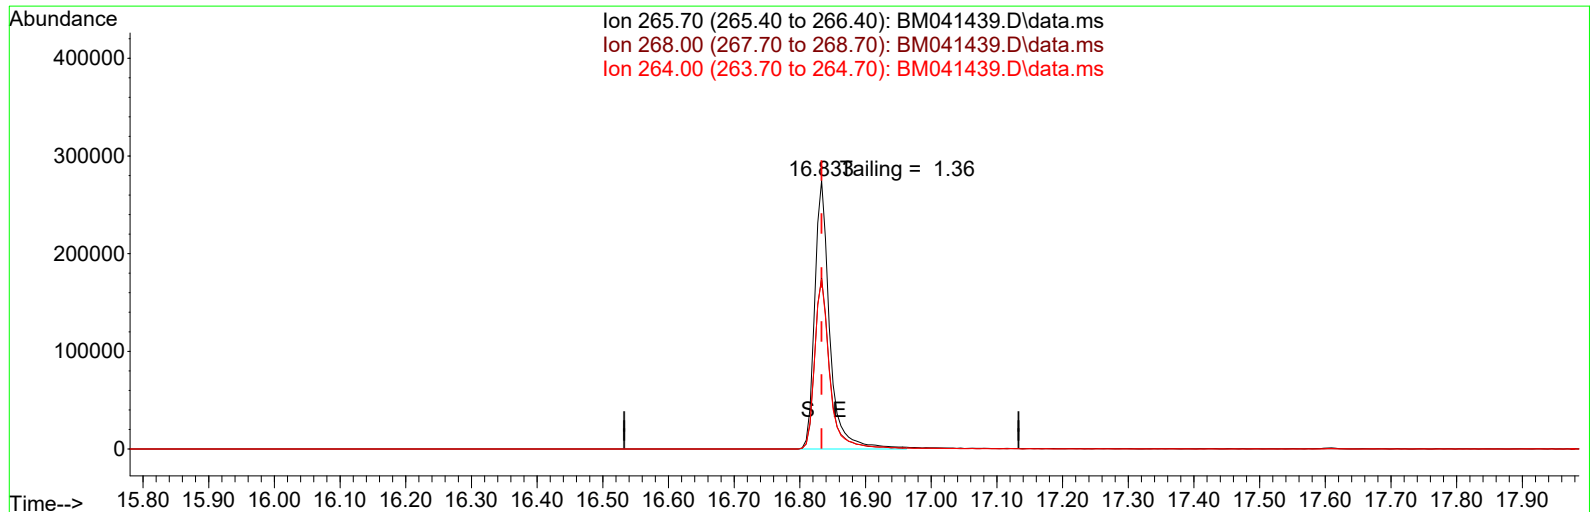

TIC: BM041439.D\data.ms

(70) Pentachlorophenol (C)




16.833min (+ 0.000) 0.00 ng

response 441686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.62
264.00	62.70	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082123\
Data File : BM041439.D
Acq On : 21 Aug 2023 09:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 04:04:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 03:32:15 2023
Response via : Initial Calibration

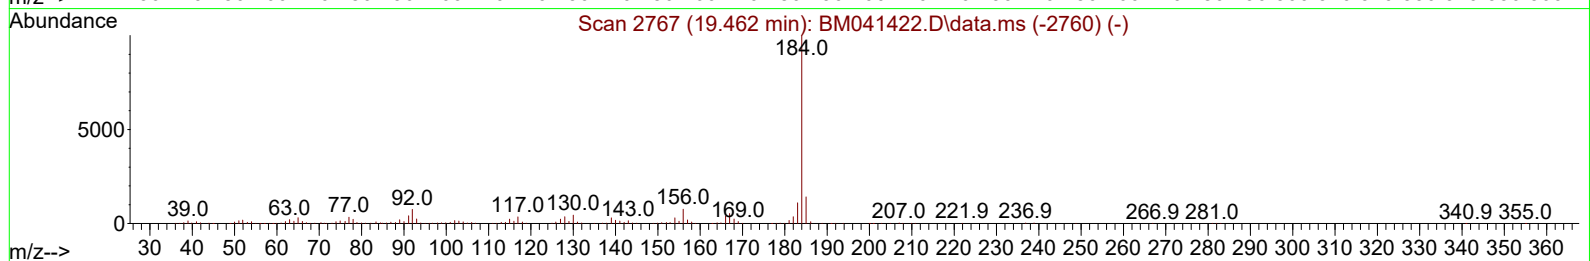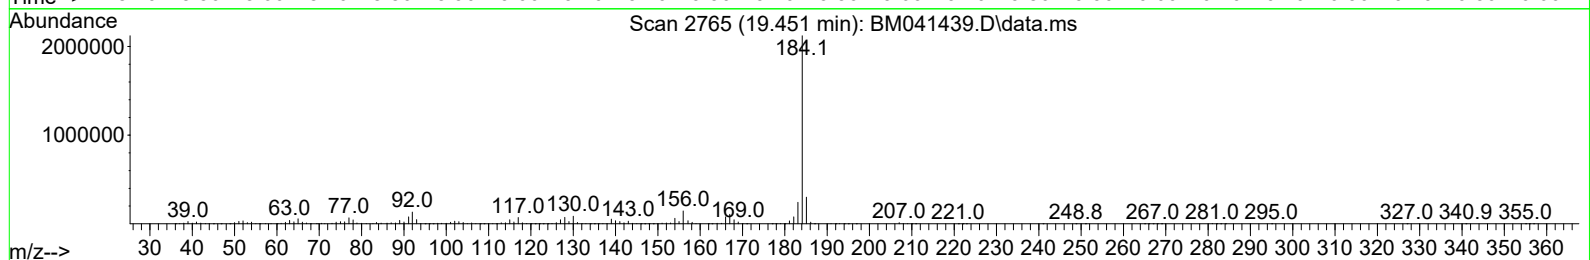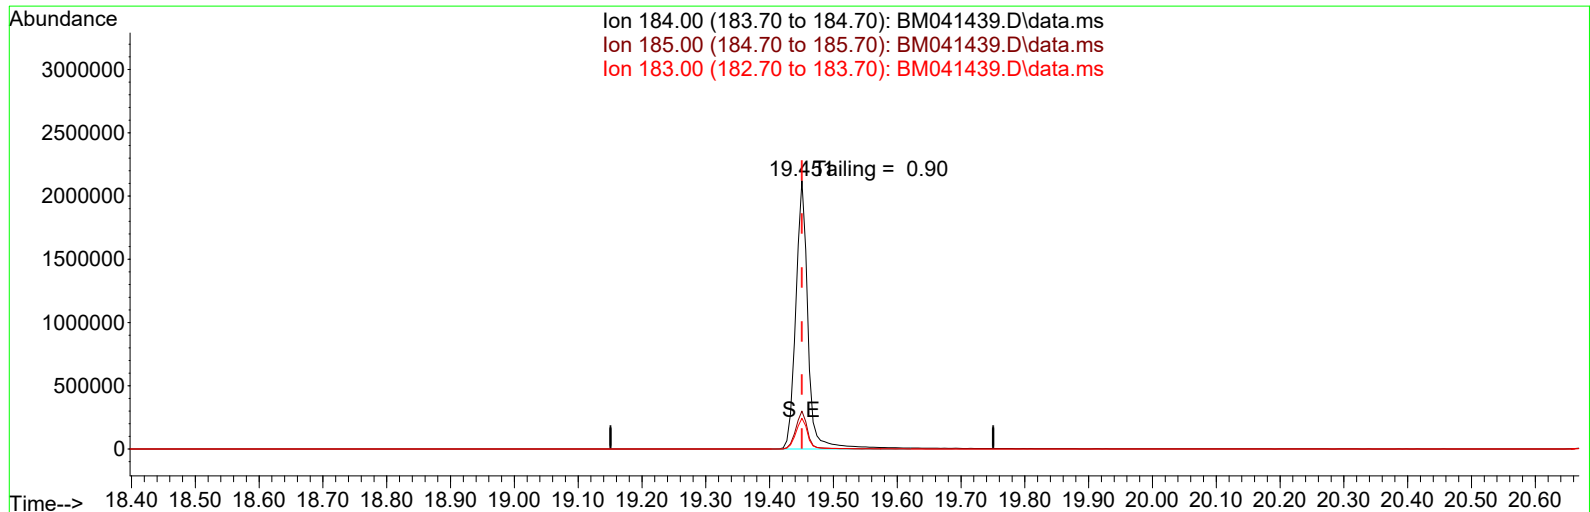

TIC: BM041439.D\data.ms

(77) Benzidine**19.451min (+ 0.000) 455063.41 ng****response 2832385**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.15
183.00	11.00	11.44
0.00	0.00	0.00