
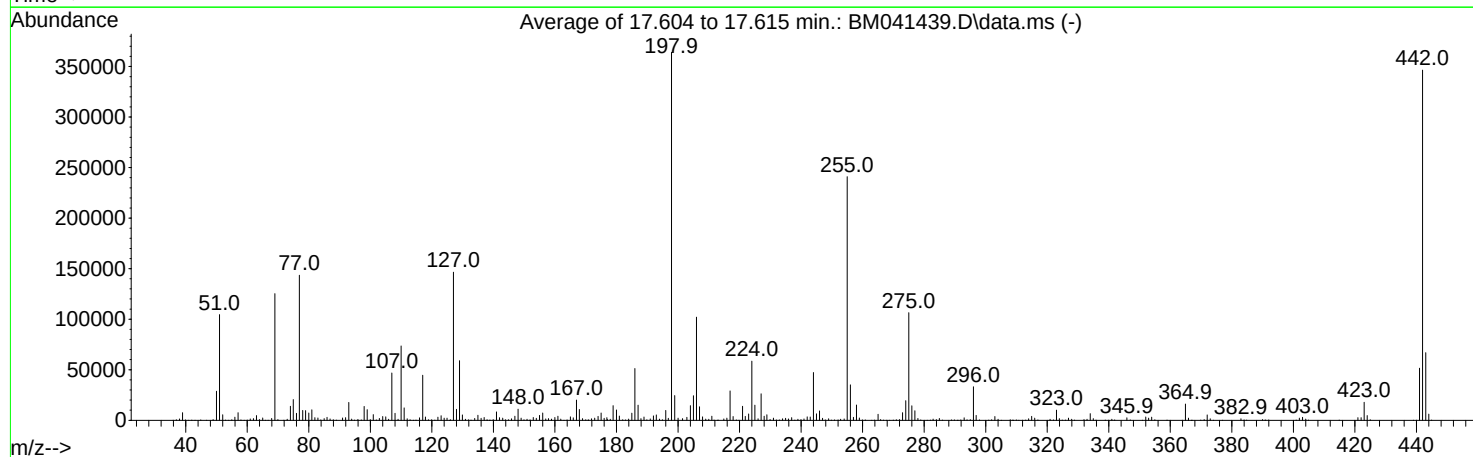


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082123\
Data File : BM041439.D
Acq On : 21 Aug 2023 09:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 22 03:32:15 2023

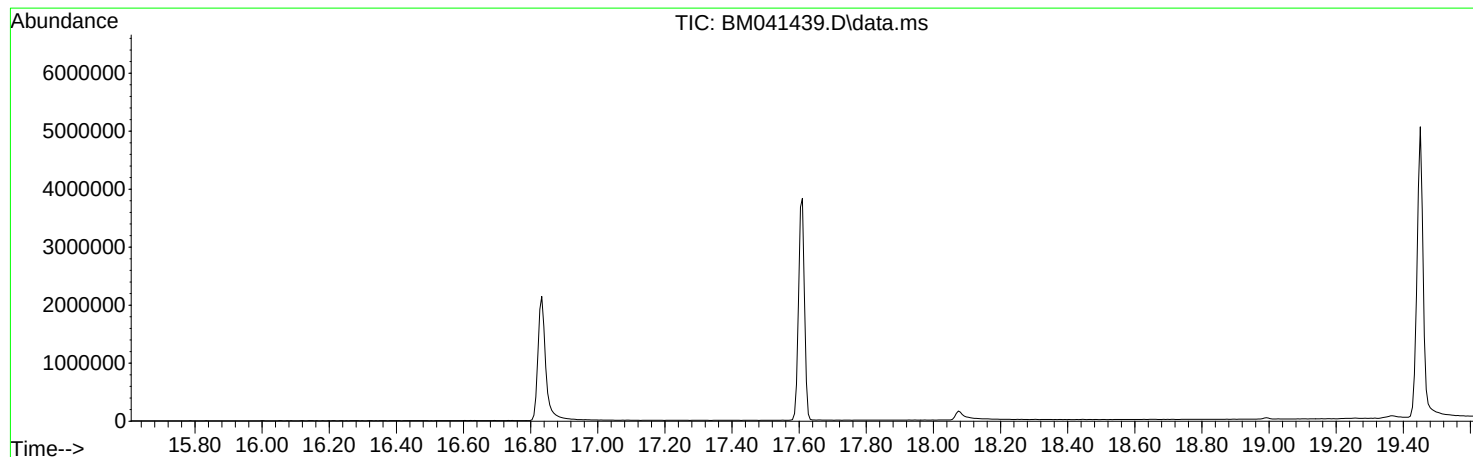




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	104510	PASS
68	69	0.00	2	1.5	1887	PASS
69	198	0.00	100	34.4	125333	PASS
70	69	0.00	2	0.5	681	PASS
127	198	10	80	40.2	146451	PASS
197	198	0.00	2	0.5	1925	PASS
198	198	100	100	100.0	363925	PASS
199	198	5	9	6.7	24504	PASS
275	198	10	60	29.3	106491	PASS
365	198	1	100	4.4	16122	PASS
441	198	0.01	100	14.2	51552	PASS
442	442	50	100	100.0	346496	PASS
443	442	15	24	19.3	66845	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082123\
Data File : BM041439.D
Acq On : 21 Aug 2023 09:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 22 04:04:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 03:32:15 2023
Response via : Initial Calibration

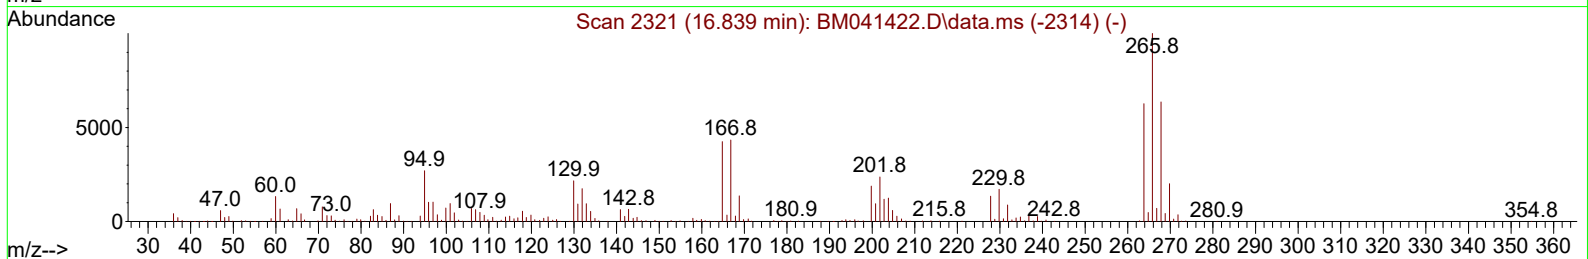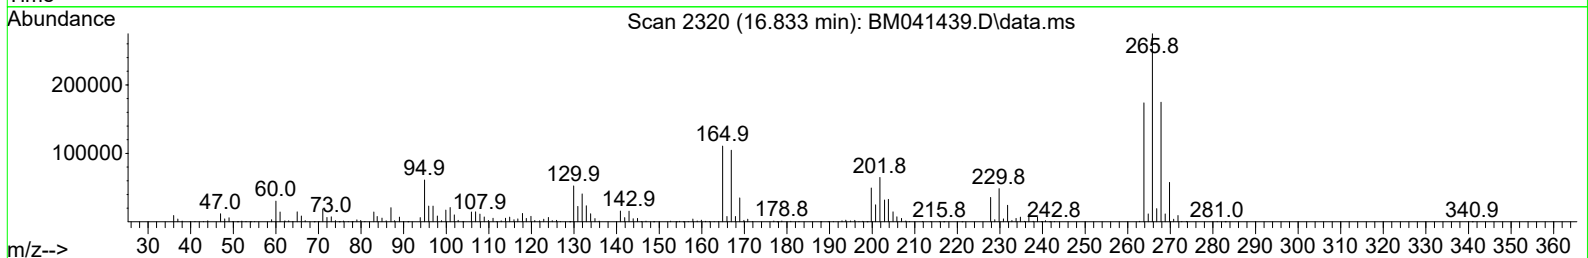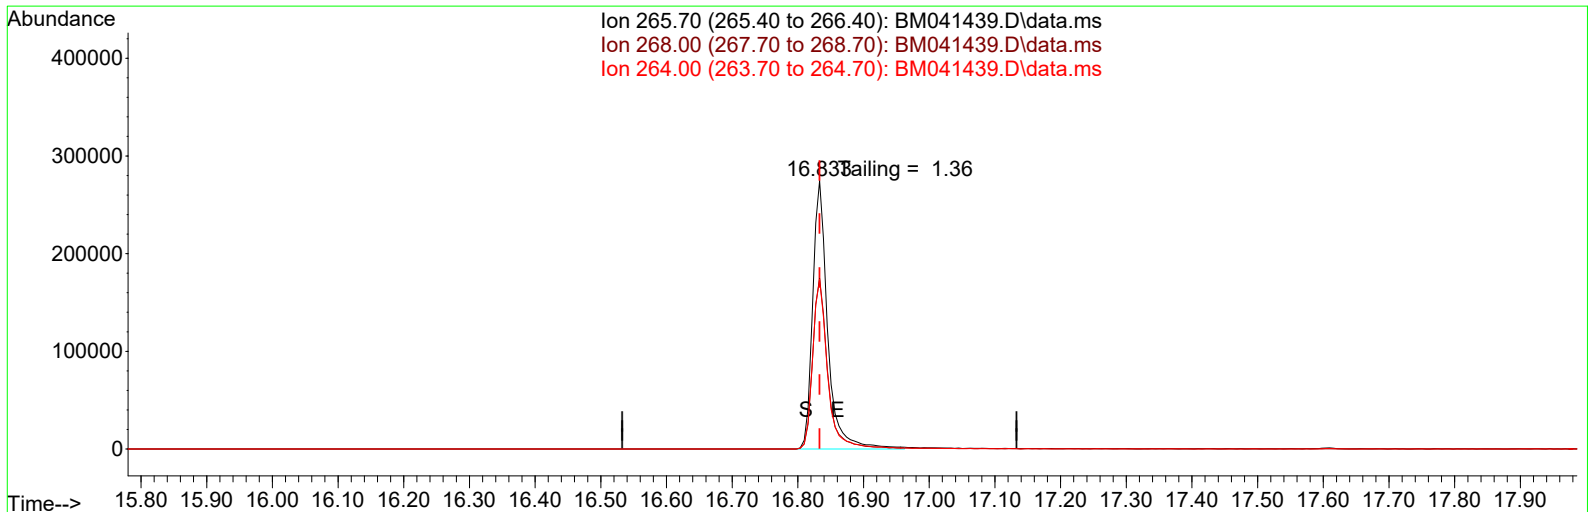

TIC: BM041439.D\data.ms

(70) Pentachlorophenol (C)

16.833min (+ 0.000) 0.00 ng




response 441686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.62
264.00	62.70	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082123\
Data File : BM041439.D
Acq On : 21 Aug 2023 09:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 22 04:04:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 03:32:15 2023
Response via : Initial Calibration

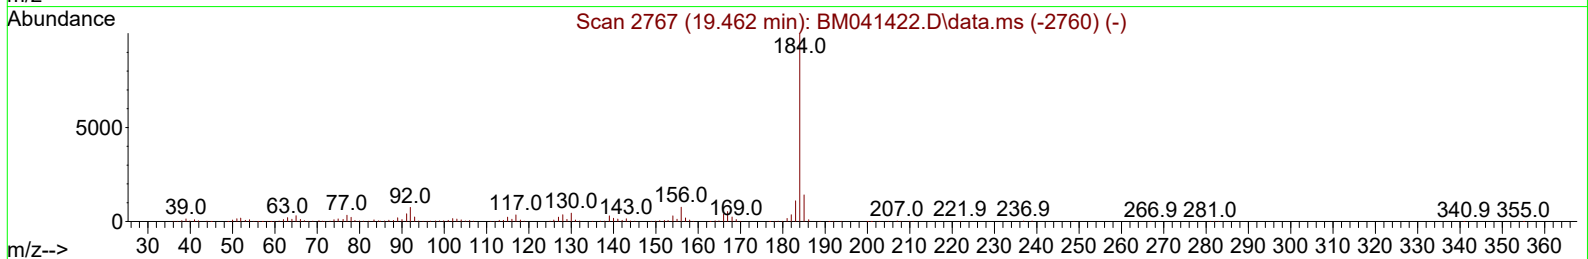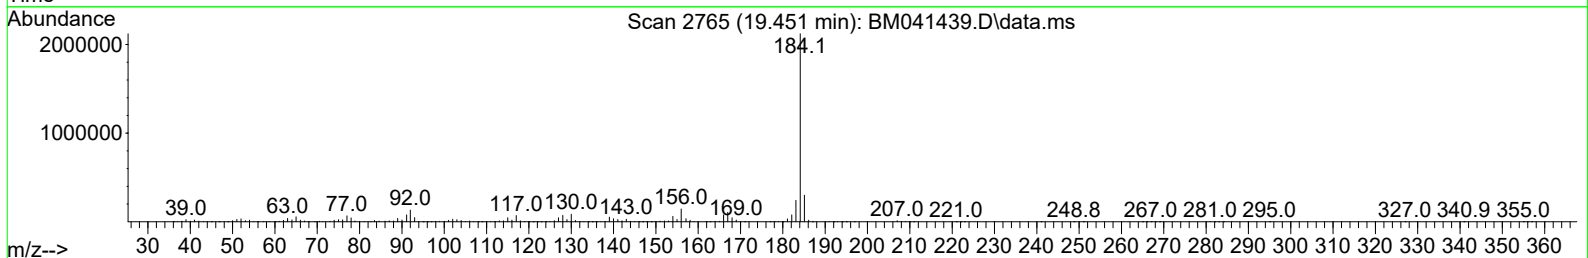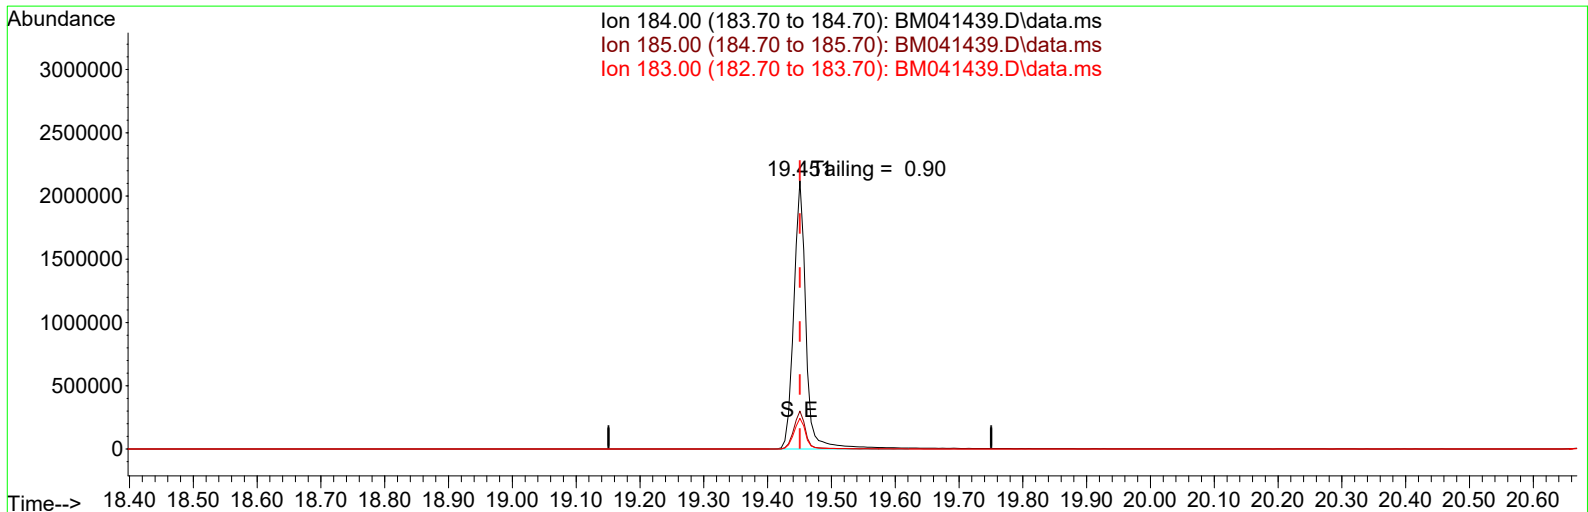

TIC: BM041439.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 455063.41 ng

response 2832385

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.15
183.00	11.00	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/21/2023	BNA_M	<u>BM041439.D</u>
Compound Name	Response	Retention Time
DDT	1530906	20.668
DDD	30862	20.233
DDE	1893	19.715
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32755	1563661	2.09

Instrument :
BNA_M
ClientSampleId :
DFTPP