
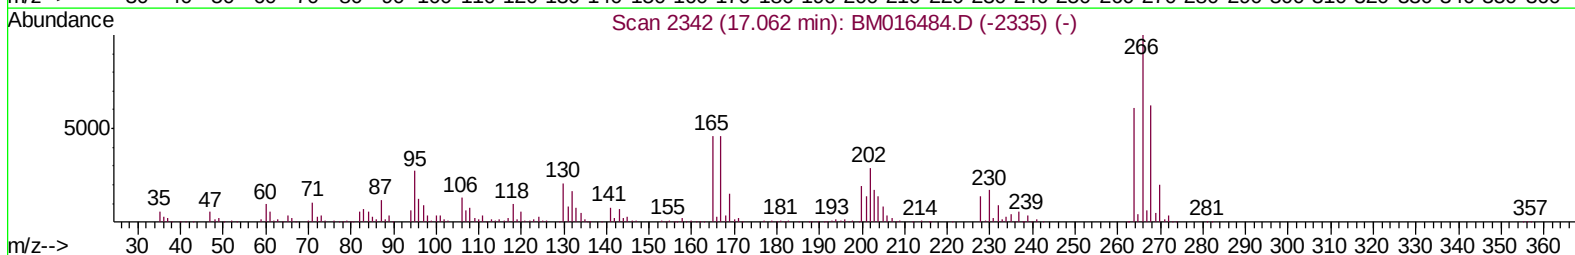
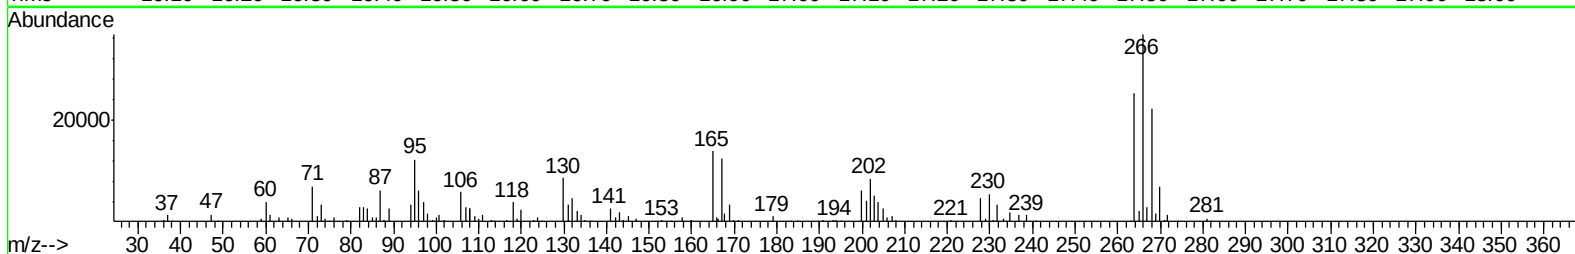


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082318\
Data File : BM016559.D
Acq On : 23 Aug 2018 18:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 07:23:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

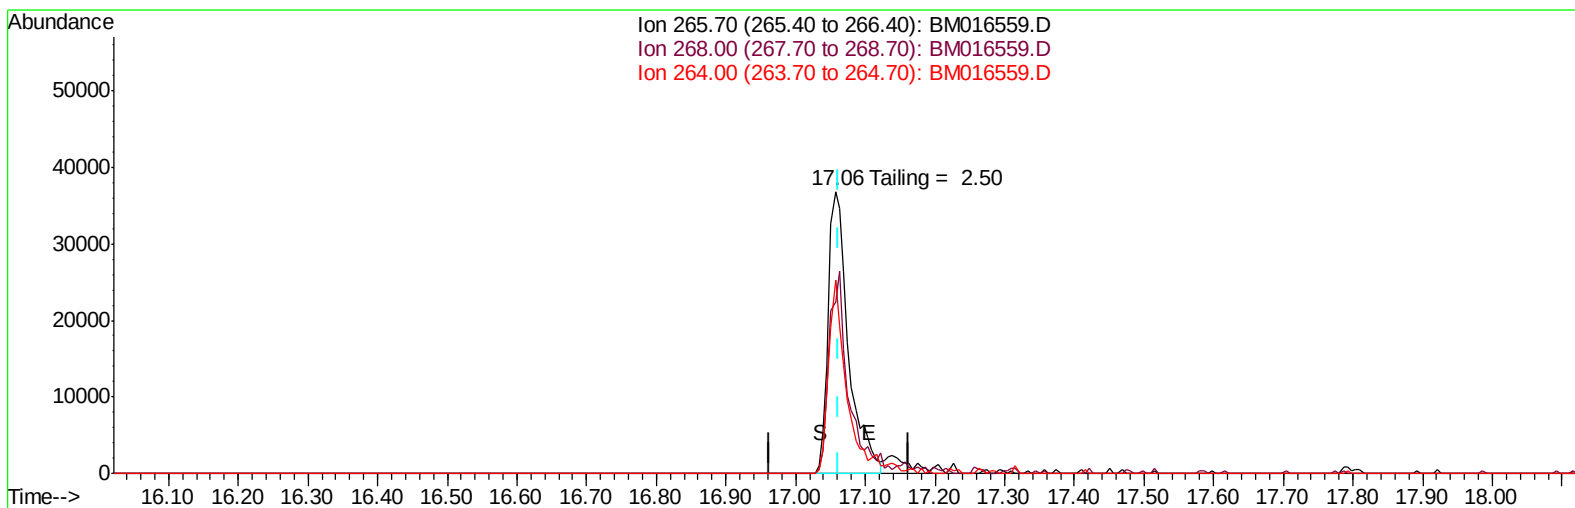

TIC: BM016559.D

(69) Pentachlorophenol (C)




17.057min (-0.006) 0.00ng

response 74450

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.76
264.00	61.20	68.46
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082318\
Data File : BM016559.D
Acq On : 23 Aug 2018 18:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 07:23:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

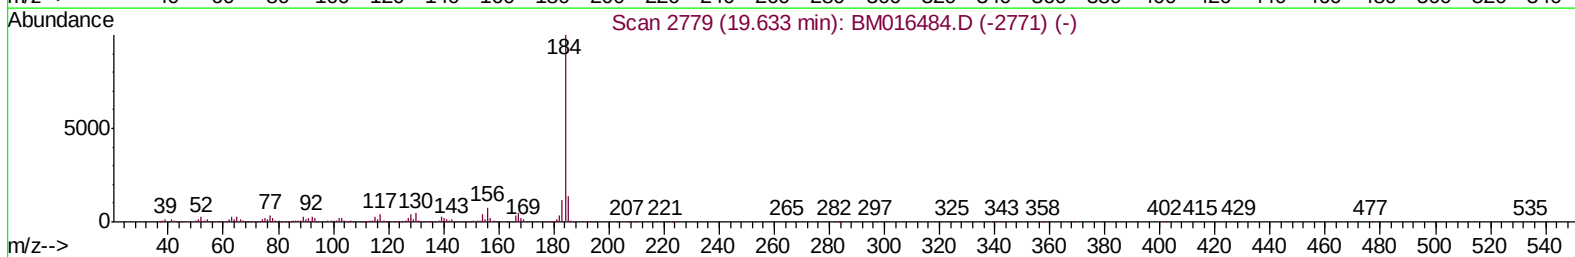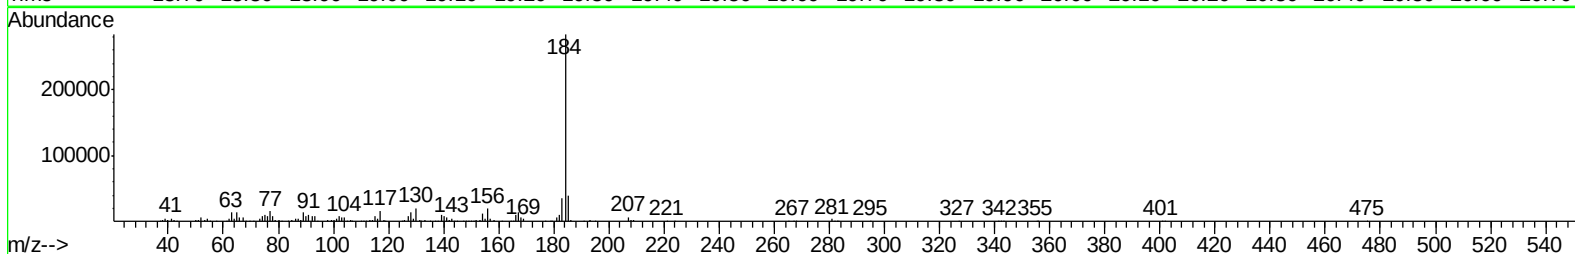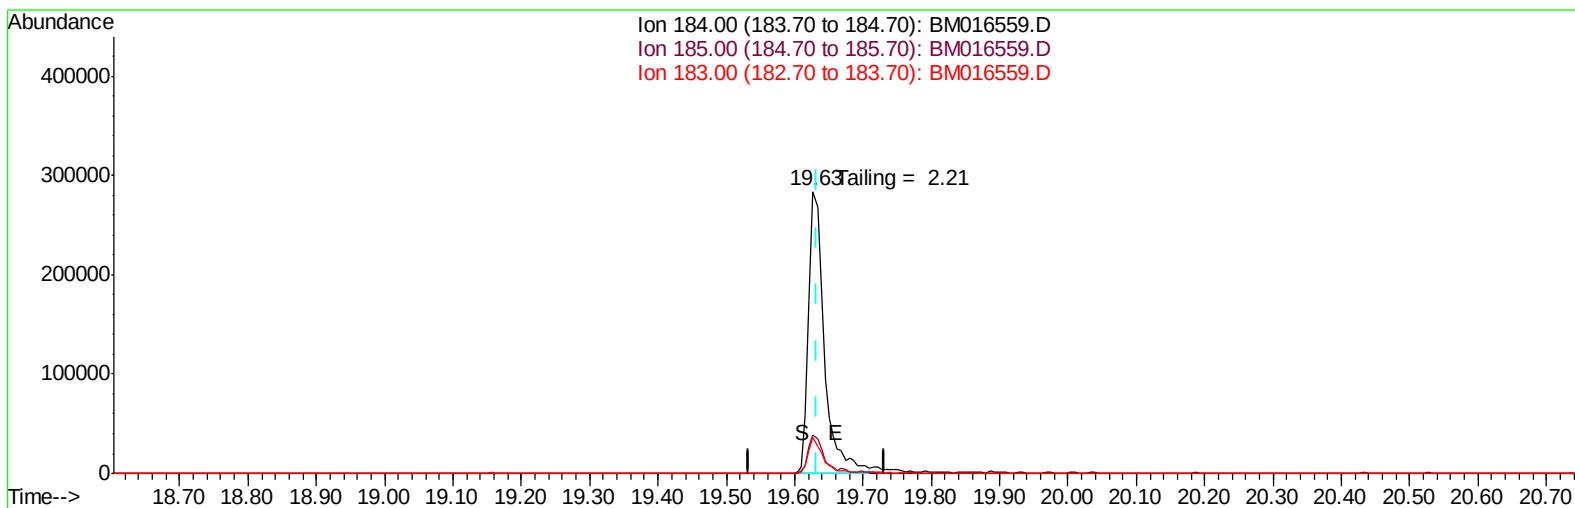

TIC: BM016559.D

(76) Benzidine

19.627min (-0.006) 153822.08ng

response 452599

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.65
183.00	11.10	12.62
0.00	0.00	0.00