

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
 Data File : BM016563.D
 Acq On : 23 Aug 2018 21:58
 Operator : SJ/JU
 Sample : PB112325BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112325BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	380	385	407	rBV	2143364	3342879	12.28%	4.062%
2	7.187	657	663	681	rBV	2157669	3422113	12.57%	4.158%
3	7.539	716	723	741	rBV	2578133	4225142	15.52%	5.134%
4	8.010	797	803	821	rBV	601215	1094971	4.02%	1.330%
5	8.328	850	857	874	rBV	3583451	5769153	21.19%	7.010%
6	9.198	998	1005	1025	rBV	1987878	3420085	12.56%	4.156%
7	10.816	1274	1280	1295	rBV	612939	1175887	4.32%	1.429%
8	13.269	1690	1697	1716	rBV	9911412	13013778	47.79%	15.812%
9	14.651	1926	1932	1945	rBV2	1130528	1796722	6.60%	2.183%
10	16.145	2180	2186	2207	rBV	5962164	8154355	29.95%	9.908%
11	17.392	2393	2398	2412	rBV	1854227	2768771	10.17%	3.364%
12	19.986	2833	2839	2852	rBV	26173284	27230255	100.00%	33.086%
13	21.539	3098	3103	3114	rBV	2650334	3587192	13.17%	4.359%
14	23.821	3485	3491	3507	rVB	1531968	3300811	12.12%	4.011%


Sum of corrected areas: 82302114

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016563.D
Acq On : 23 Aug 2018 21:58
Operator : SJ/JU
Sample : PB112325BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

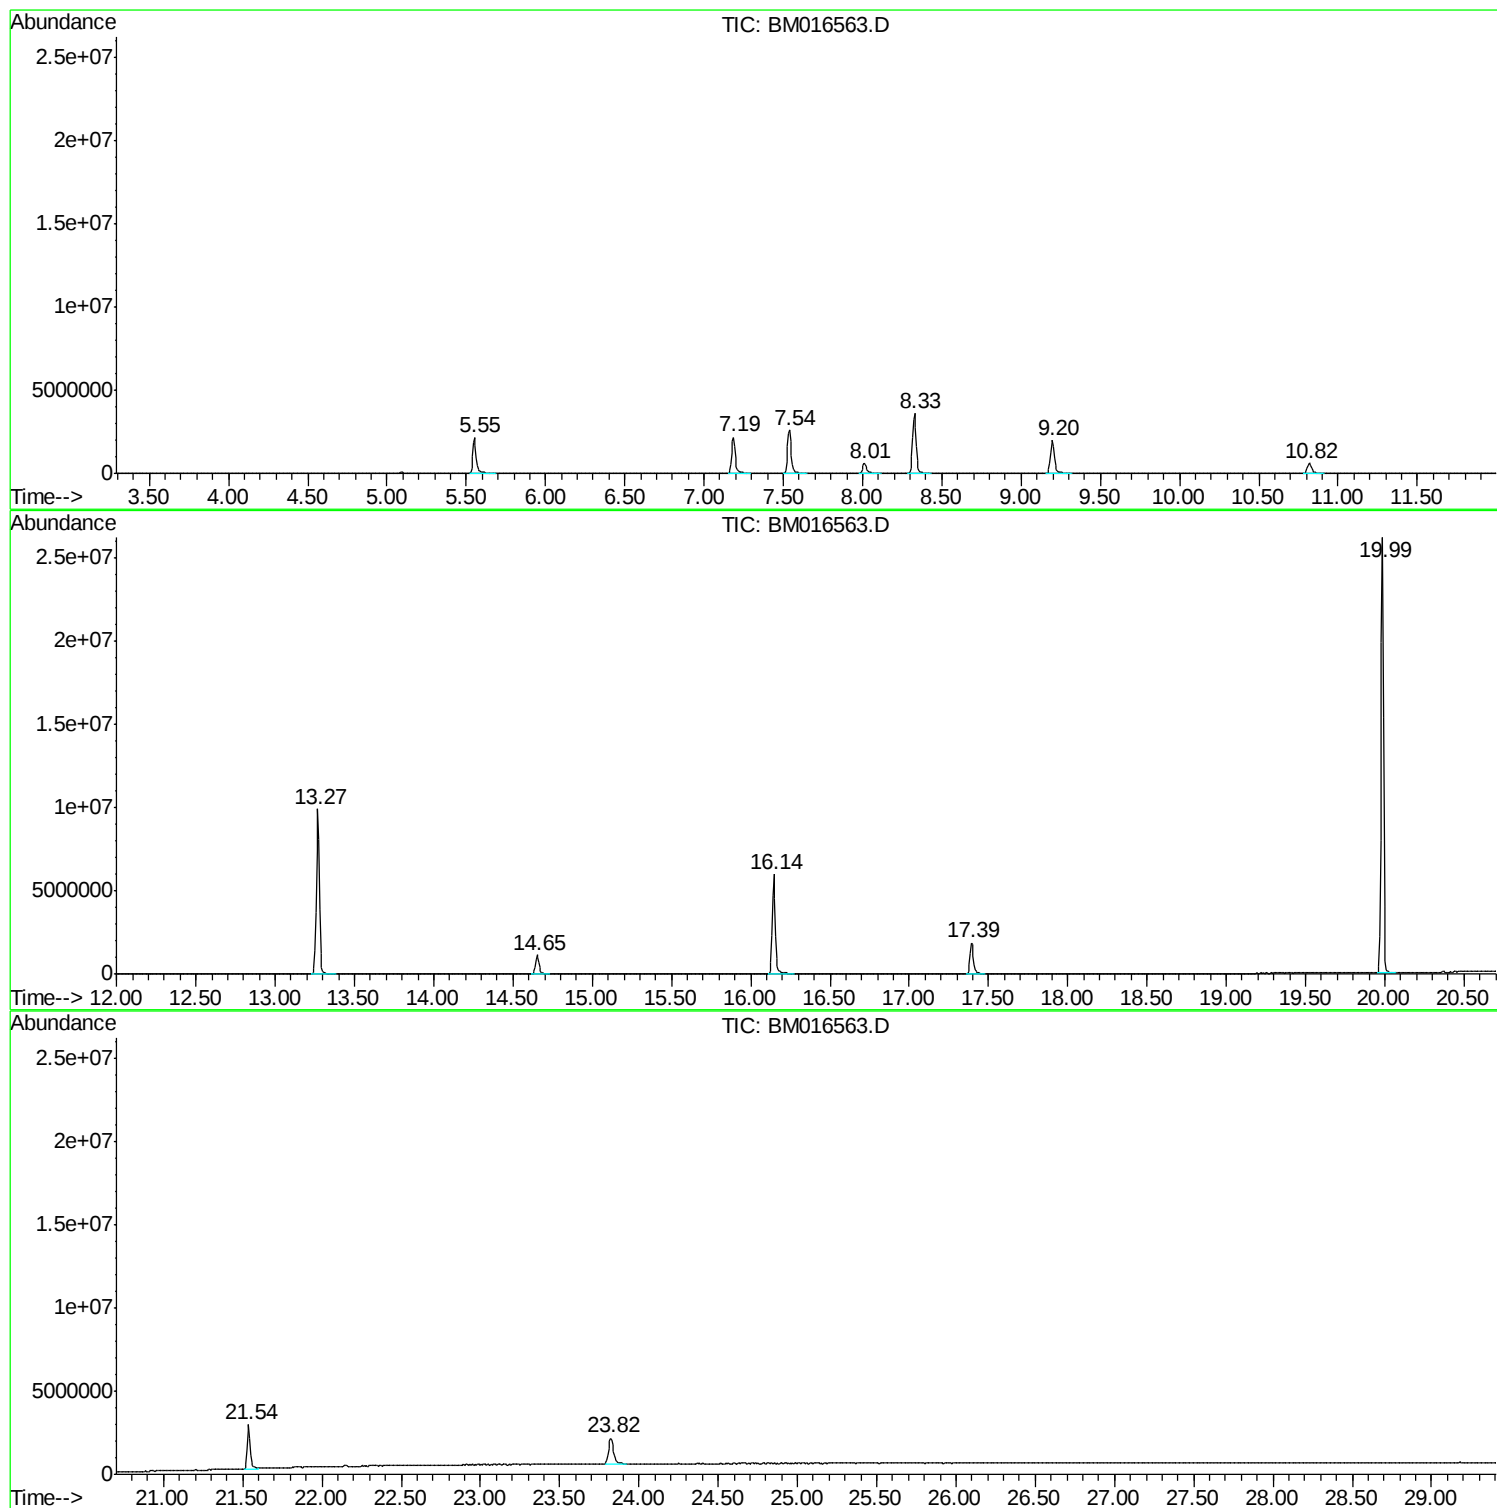

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016563.D
Acq On : 23 Aug 2018 21:58
Operator : SJ/JU
Sample : PB112325BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112325BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	77.17 ng	4225140	1,4-Dichlorobenzene-d4	8.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	12
2		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

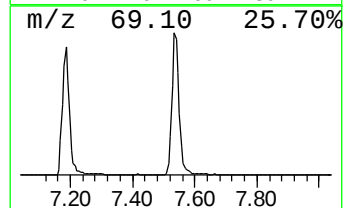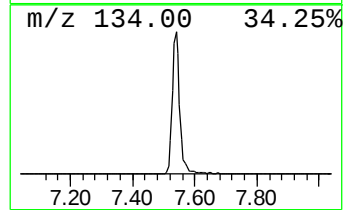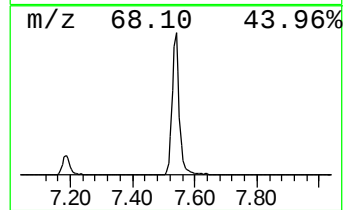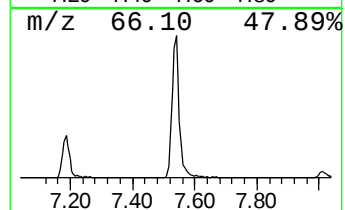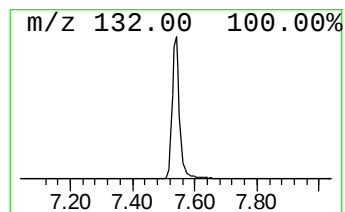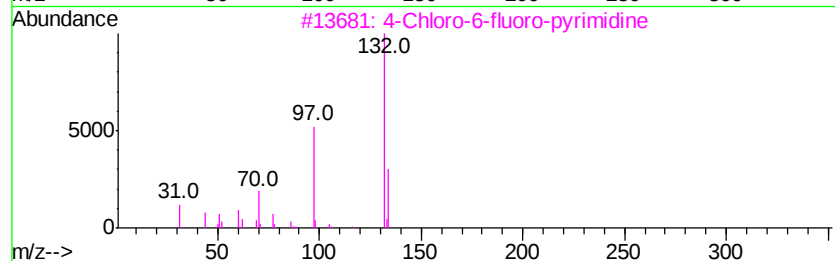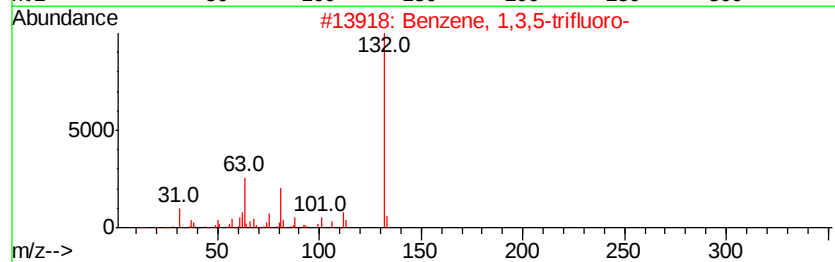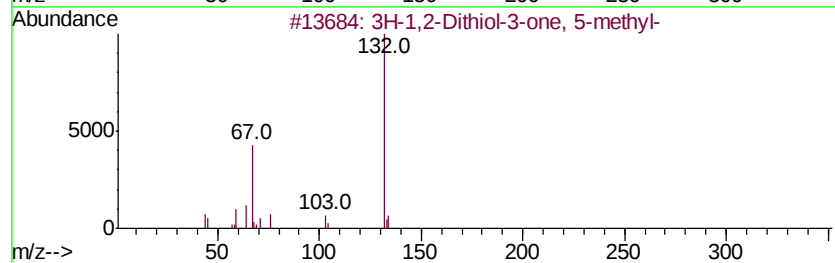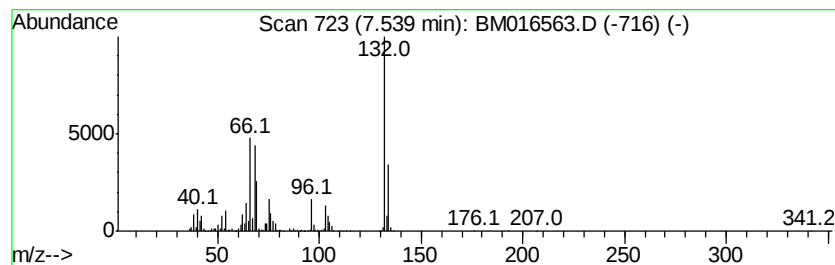

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082318\
Data File : BM016563.D
Acq On : 23 Aug 2018 21:58
Operator : SJ/JU
Sample : PB112325BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.54	7.54	77.2	ng	4225140	1	8.01	1094970	20.0