

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
 Data File : BM016567.D
 Acq On : 24 Aug 2018 00:22
 Operator : SJ/JU
 Sample : J4610-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 082118-DBRI-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	381	385	407	rBV	476803	939753	4.37%	1.525%
2	7.186	658	663	686	rBV2	304559	606956	2.82%	0.985%
3	7.539	717	723	742	rBV	1396022	2469289	11.49%	4.007%
4	8.010	797	803	819	rBV	425590	801589	3.73%	1.301%
5	8.328	850	857	871	rBV	2790149	4471499	20.81%	7.256%
6	9.198	998	1005	1021	rBV	1515178	2709818	12.61%	4.397%
7	10.816	1273	1280	1292	rBV	451388	873935	4.07%	1.418%
8	13.268	1690	1697	1711	rBV	7913708	10238708	47.65%	16.614%
9	14.651	1923	1932	1942	rBV3	855559	1408654	6.56%	2.286%
10	16.145	2180	2186	2207	rBV	4919366	6939613	32.30%	11.261%
11	17.392	2393	2398	2411	rBV	1421668	2086185	9.71%	3.385%
12	19.986	2833	2839	2847	rBV	18782485	21487157	100.00%	34.867%
13	21.538	3098	3103	3111	rBV	2320582	3212735	14.95%	5.213%
14	23.821	3485	3491	3504	rBV	1686928	3380930	15.73%	5.486%


Sum of corrected areas: 61626821

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016567.D
Acq On : 24 Aug 2018 00:22
Operator : SJ/JU
Sample : J4610-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-DBRI-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

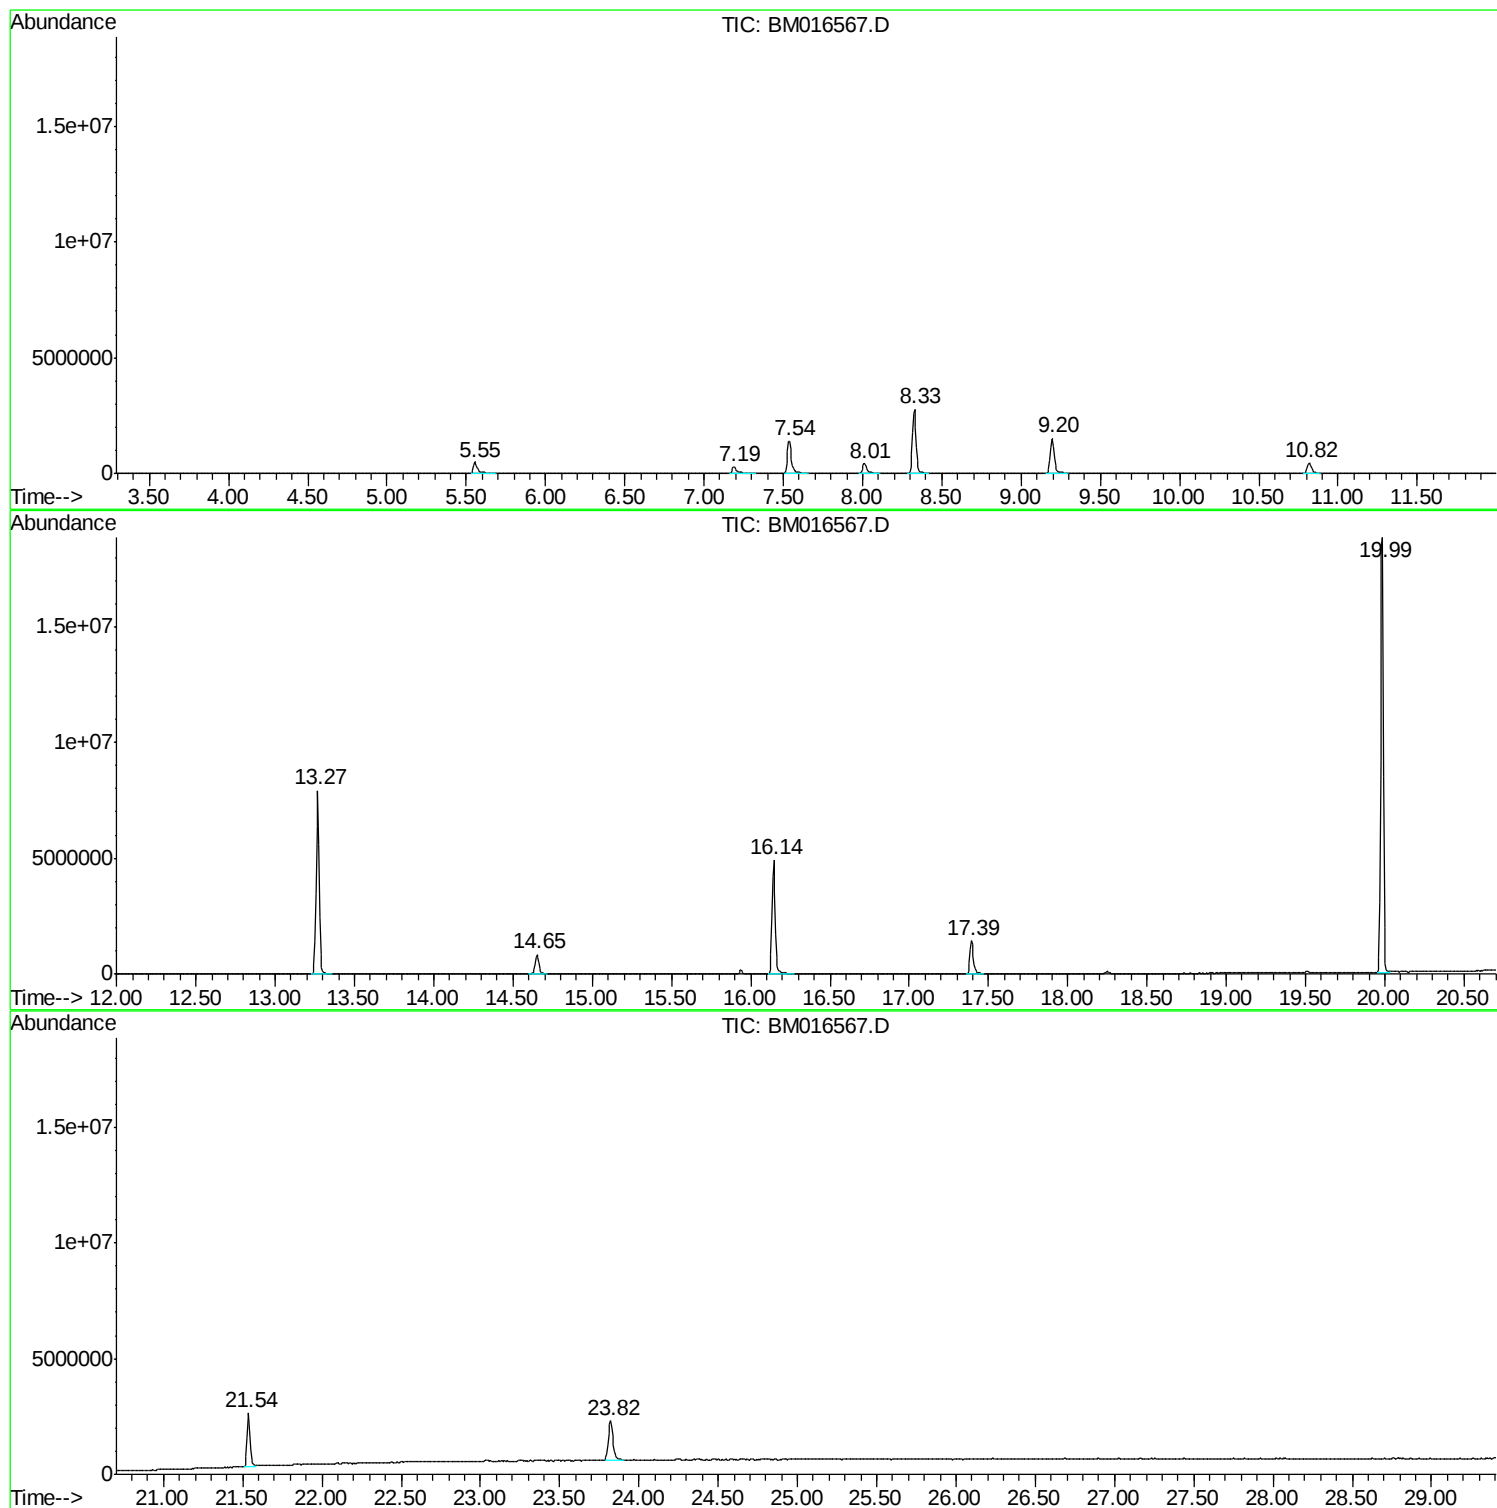

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016567.D
Acq On : 24 Aug 2018 00:22
Operator : SJ/JU
Sample : J4610-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-DBRI-F-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	61.61 ng	2469290	1,4-Dichlorobenzene-d4	8.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	11
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	10
4		3H-1,2-Dithiol-3-one, 4-methyl-	132	C4H4OS2	003620-10-8	10
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10

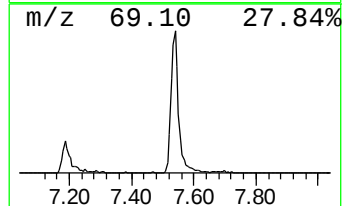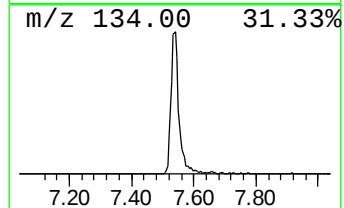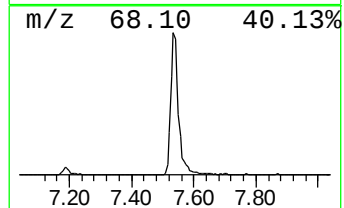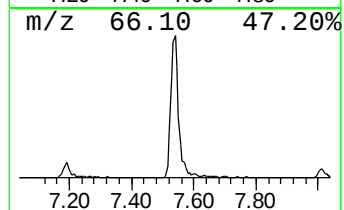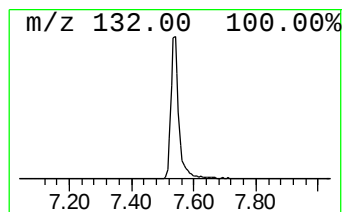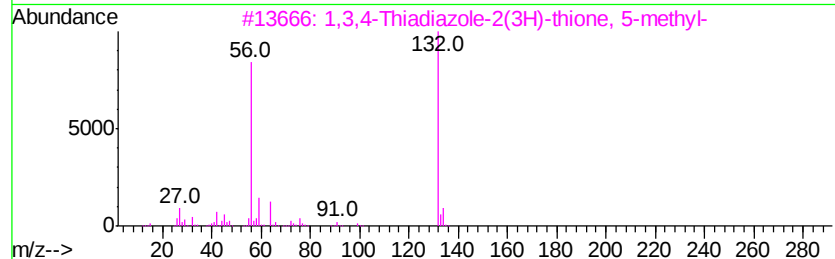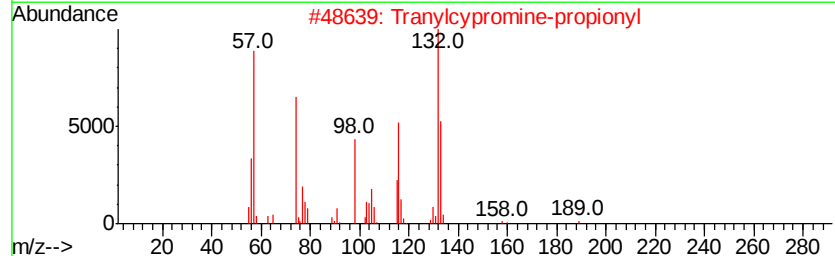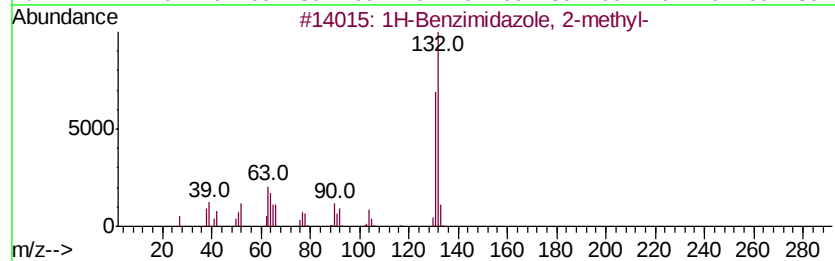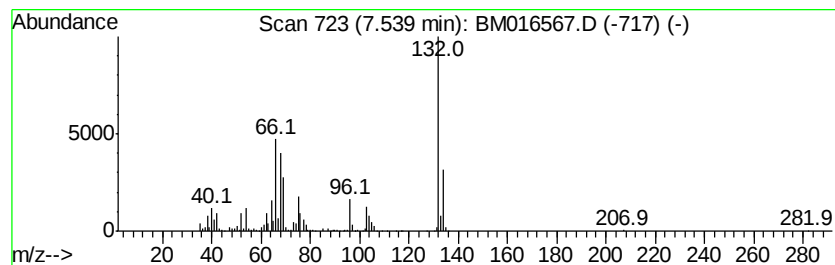

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082318\
Data File : BM016567.D
Acq On : 24 Aug 2018 00:22
Operator : SJ/JU
Sample : J4610-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-DBRI-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.54	7.54	61.6	ng	2469290	1	8.01	801589	20.0