

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
 Data File : BM016571.D
 Acq On : 24 Aug 2018 02:46
 Operator : SJ/JU
 Sample : J4610-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 082118-SIDI-E-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	381	385	403	rBV	452737	868166	4.24%	1.477%
2	7.187	659	663	677	rBV	275765	524615	2.56%	0.892%
3	7.534	716	722	740	rBV	1325552	2335695	11.40%	3.973%
4	8.010	797	803	816	rBV2	421983	780579	3.81%	1.328%
5	8.322	850	856	870	rBV	2567590	4254267	20.76%	7.237%
6	9.192	998	1004	1019	rBV	1477180	2605936	12.71%	4.433%
7	10.816	1274	1280	1294	rBV	473541	884903	4.32%	1.505%
8	13.269	1690	1697	1712	rBV	7202522	9655568	47.11%	16.426%
9	14.651	1923	1932	1946	rBV2	850183	1409405	6.88%	2.398%
10	16.145	2180	2186	2204	rBV	4608928	6432473	31.38%	10.943%
11	17.392	2393	2398	2412	rBV	1360334	2053939	10.02%	3.494%
12	19.980	2833	2838	2846	rBV	17612130	20496176	100.00%	34.867%
13	21.539	3098	3103	3112	rBV	2288674	3145741	15.35%	5.351%
14	23.815	3485	3490	3503	rVB	1581751	3336027	16.28%	5.675%


Sum of corrected areas: 58783490

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016571.D
Acq On : 24 Aug 2018 02:46
Operator : SJ/JU
Sample : J4610-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-SIDI-E-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

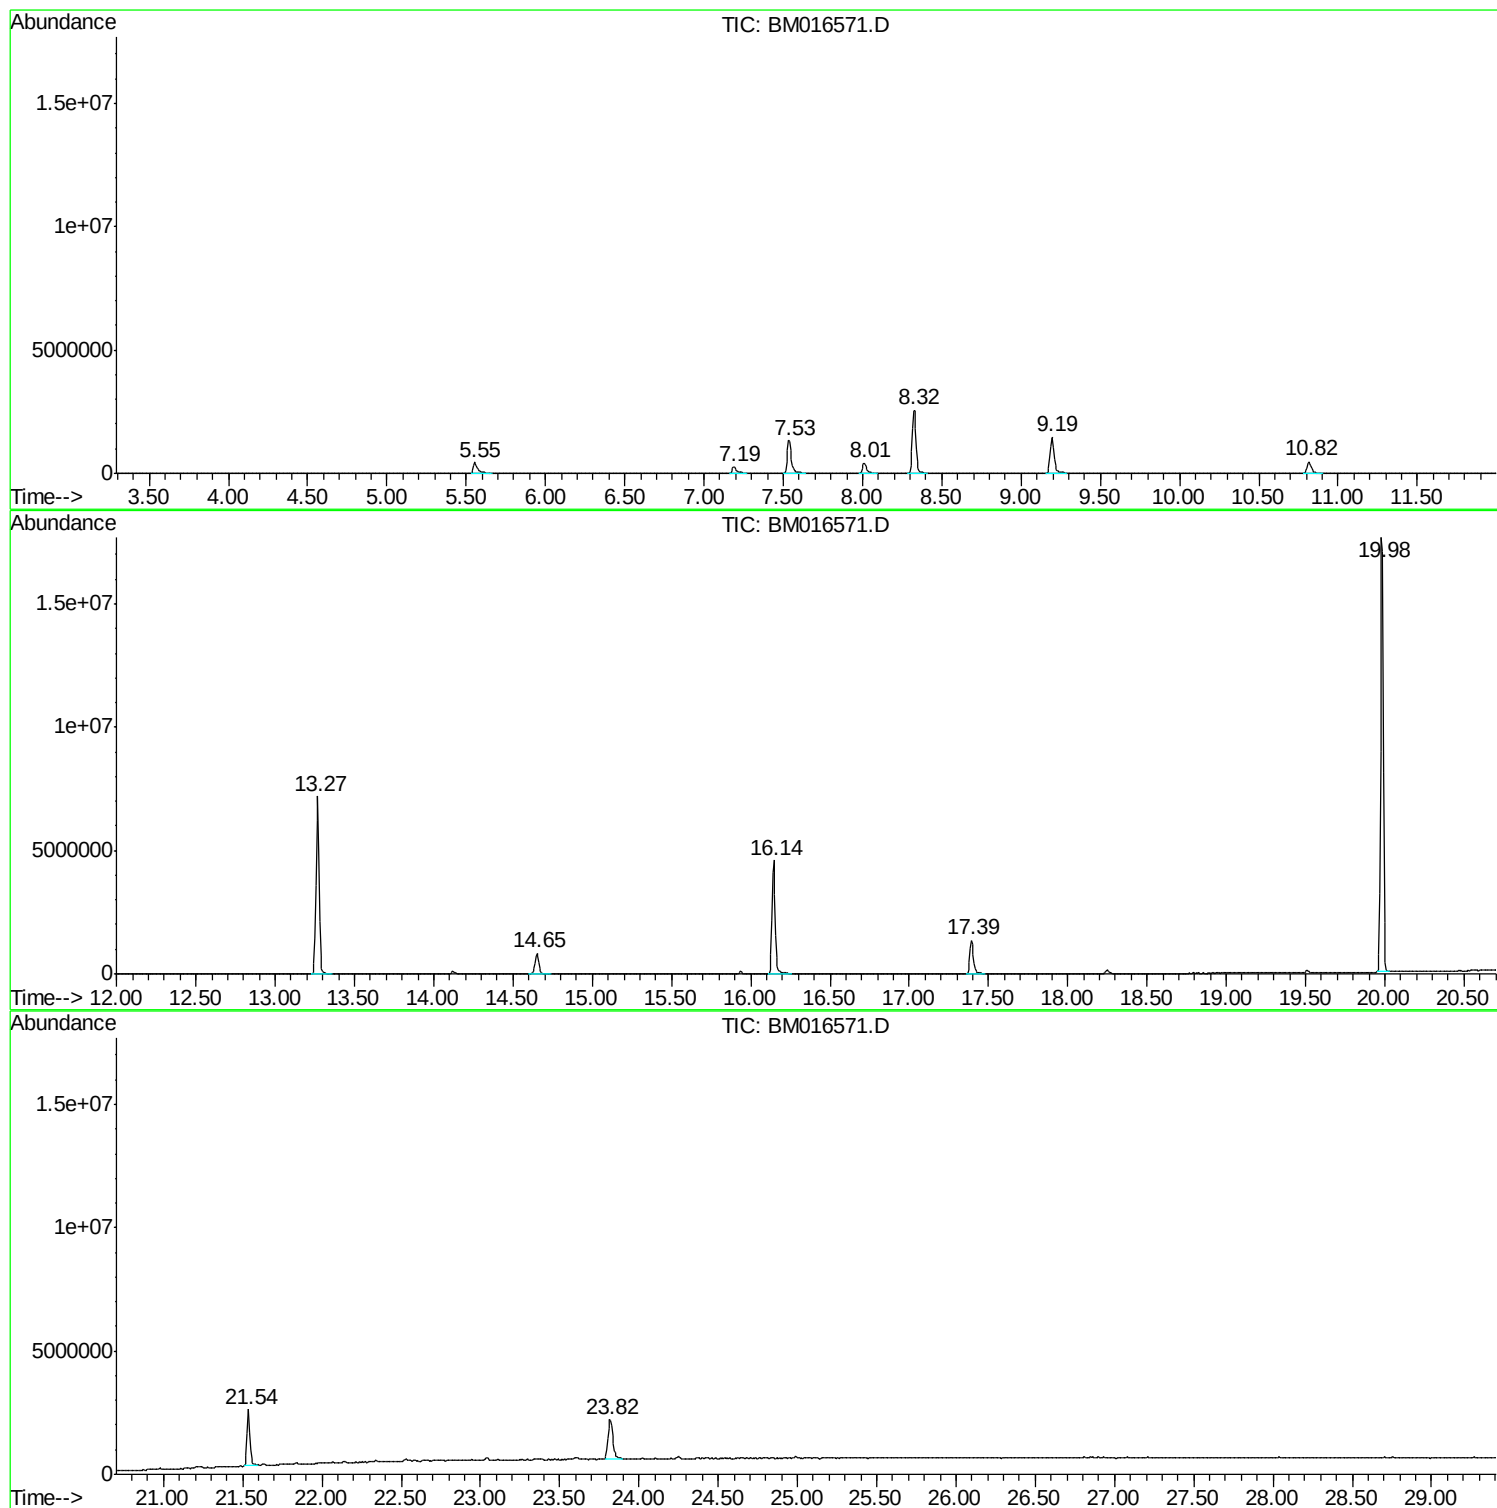

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082318\
Data File : BM016571.D
Acq On : 24 Aug 2018 02:46
Operator : SJ/JU
Sample : J4610-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-SIDI-E-D-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.53 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.53	59.85 ng	2335700	1,4-Dichlorobenzene-d4	8.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentadiene	66	C5H6	000542-92-7	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	22
3		1,4,4a,8a-Tetrahydro-1,4-methano...	174	C11H10O2	001200-89-1	16
4		Tricyclo[4.2.1.0<2,5>]non-3-ene	120	C9H12	007078-40-2	16
5		3-Hexenedinitrile	106	C6H6N2	001119-85-3	16

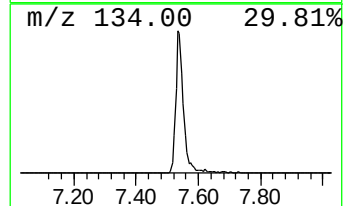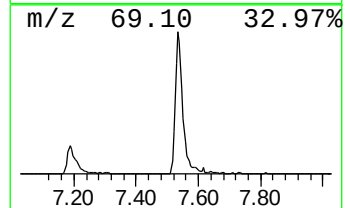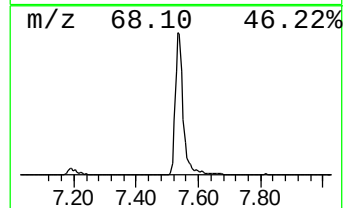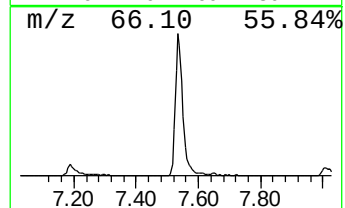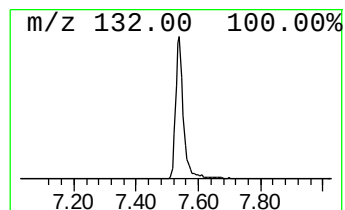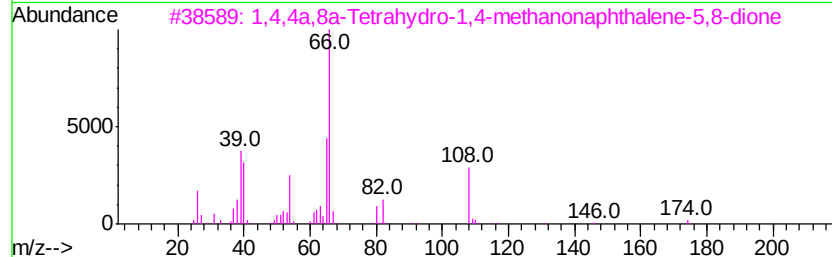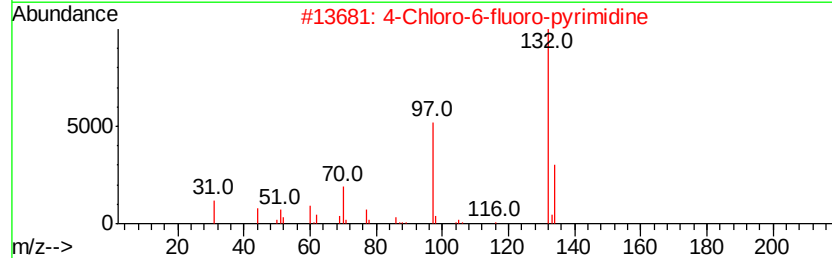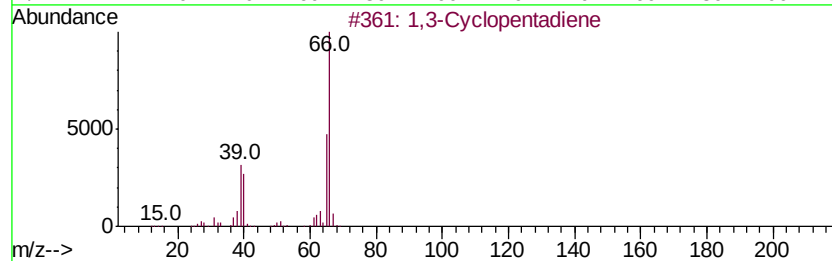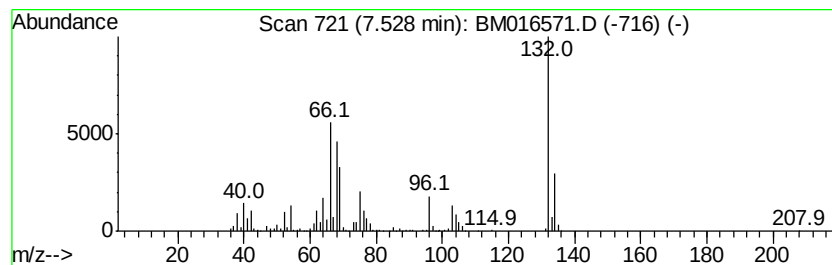

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082318\
Data File : BM016571.D
Acq On : 24 Aug 2018 02:46
Operator : SJ/JU
Sample : J4610-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
082118-SIDI-E-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.53	7.53	59.9	ng	2335700	1	8.01	780579	20.0