


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082318\  
 Data File : BM016559.D  
 Acq On : 23 Aug 2018 18:57  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM082118.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Aug 24 10:59:20 2018

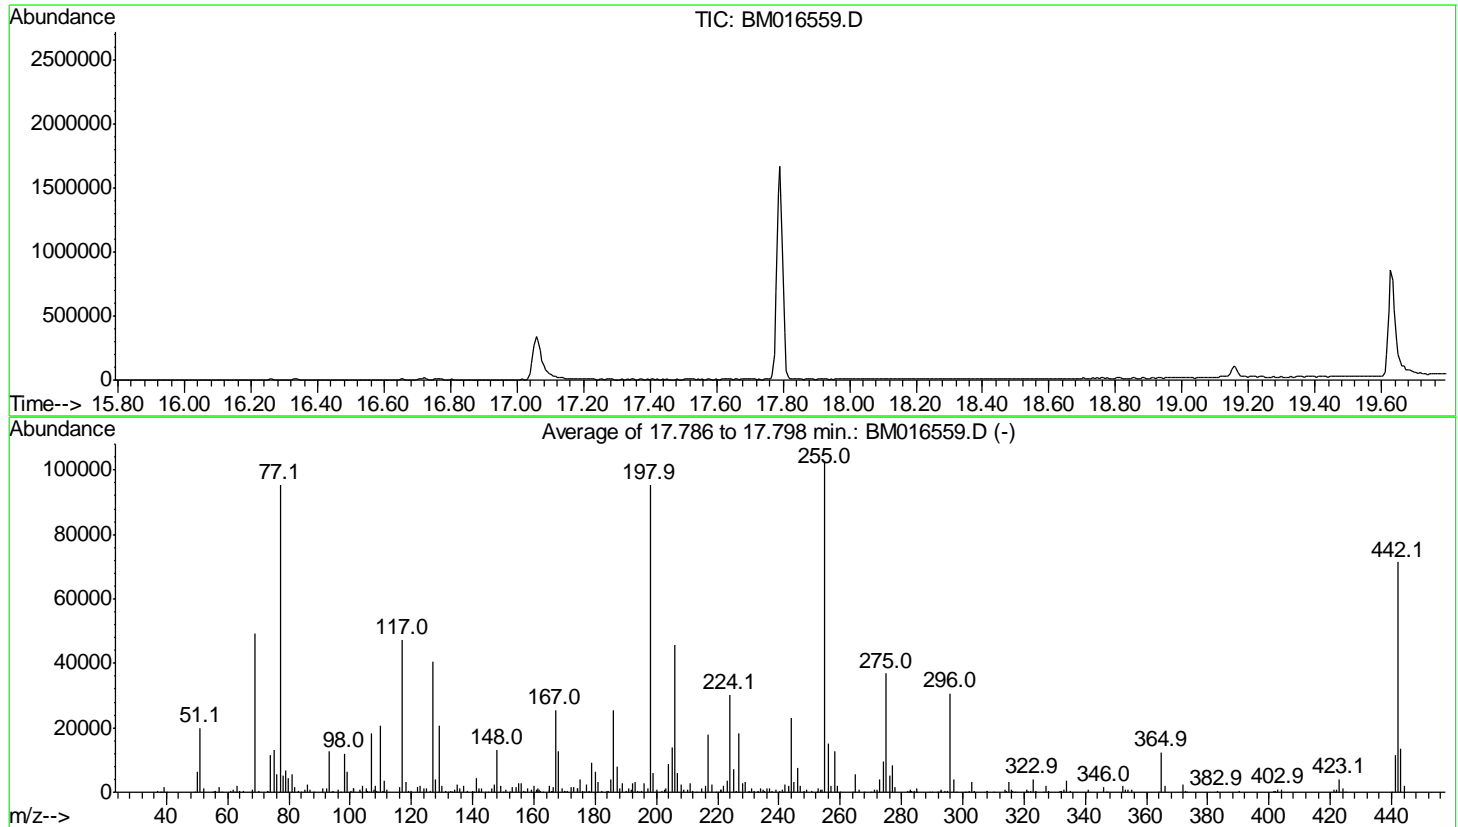

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	20004	PASS
68	69	0.00	2	1.7	857	PASS
69	198	0.00	100	51.8	49445	PASS
70	69	0.00	2	1.1	525	PASS
127	198	10	80	42.4	40466	PASS
197	198	0.00	2	1.1	1049	PASS
198	198	100	100	100.0	95480	PASS
199	198	5	9	6.3	6017	PASS
275	198	10	60	38.6	36848	PASS
365	198	1	100	13.0	12371	PASS
441	198	0.01	100	12.0	11469	PASS
442	198	50	100	74.9	71474	PASS
443	442	15	24	18.7	13370	PASS