
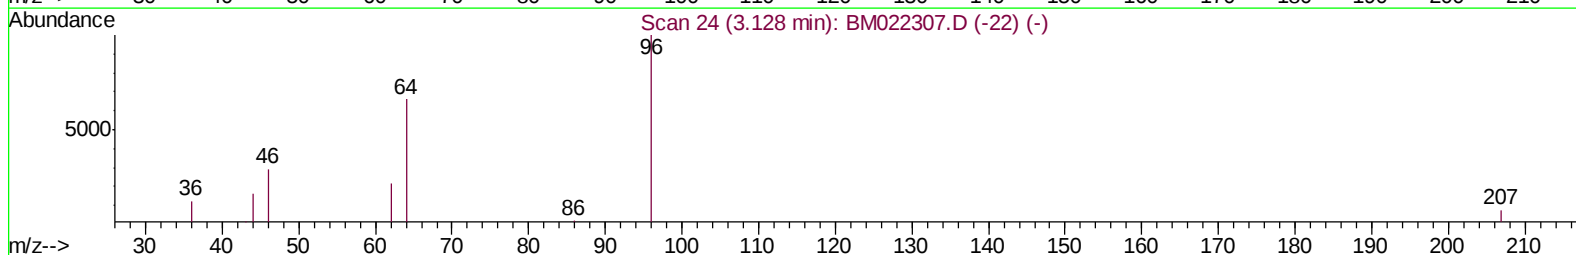
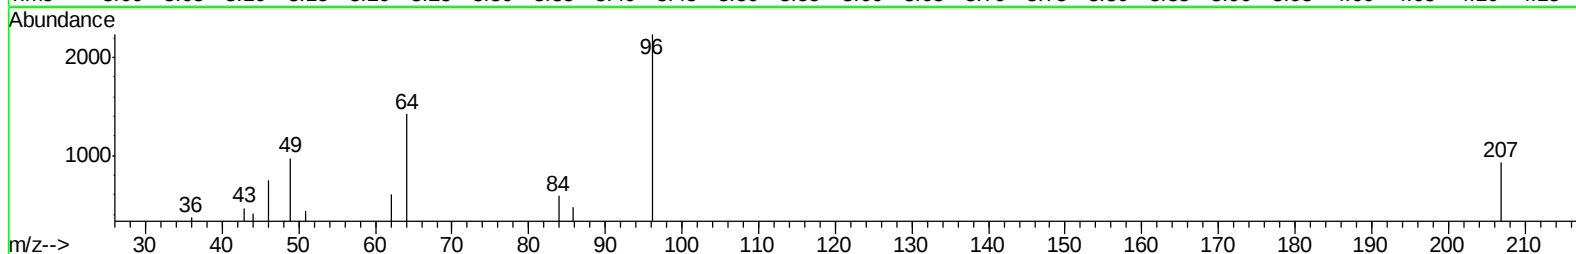


Data File : BM022308.D
Acq On : 25 Aug 2019 01:05
Operator : HP/JU
Sample : K4373-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 26 01:35:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

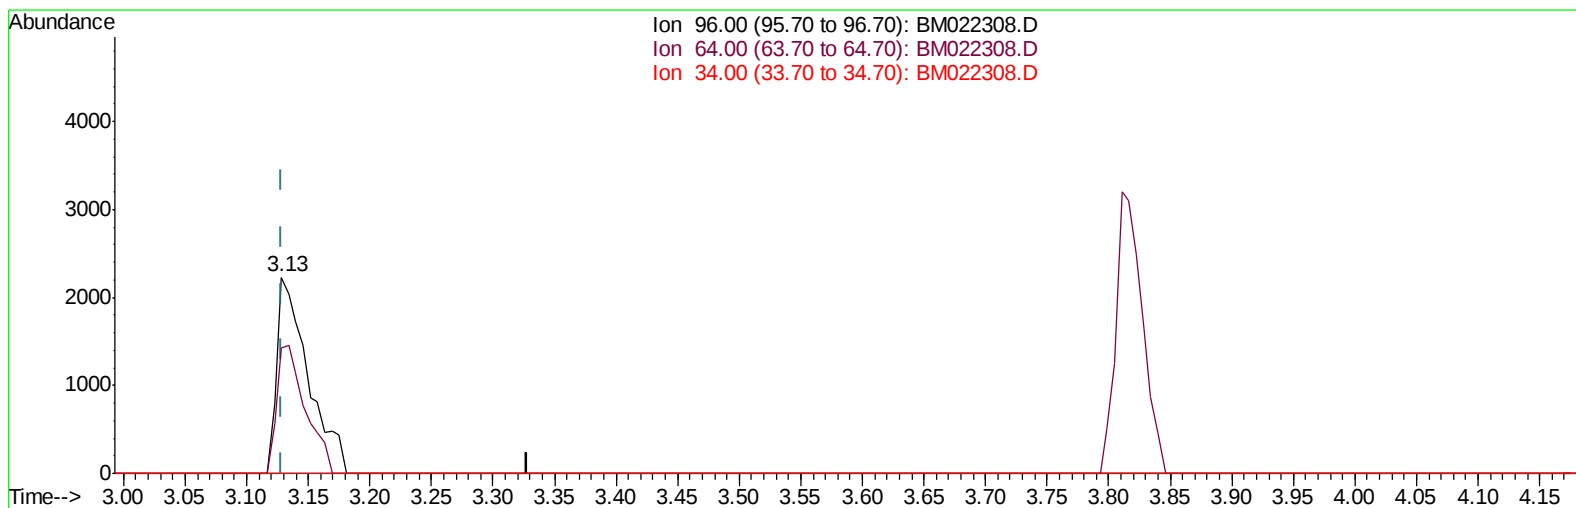

TIC: BM022308.D

(3) 1,4-Dioxane-d8 (S)

3.128min (+0.000) 4.43ng/uL m

response 4000

Ion	Exp%	Act%
96.00	100	100
64.00	64.80	63.64
34.00	0.00	0.00
0.00	0.00	0.00