
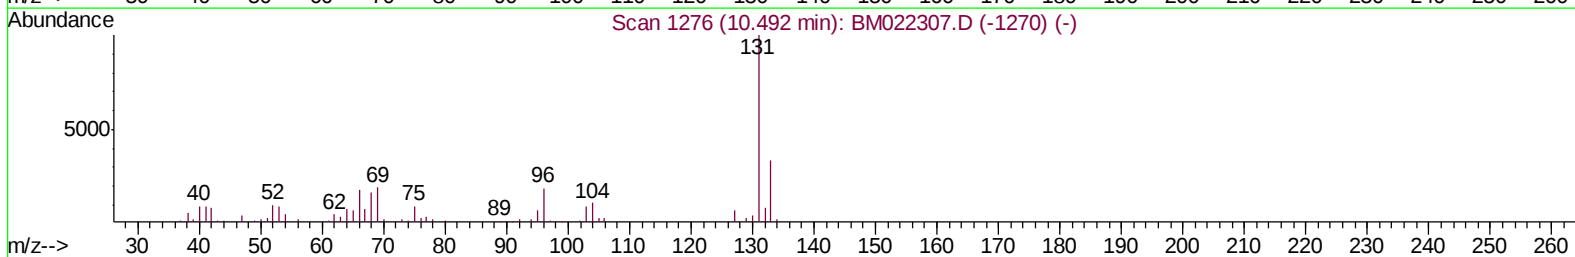
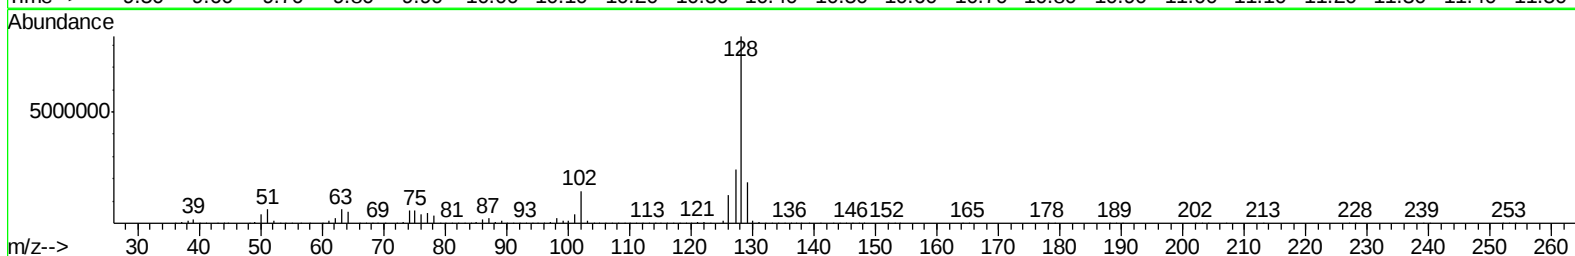


Data File : BM022308.D
Acq On : 25 Aug 2019 01:05
Operator : HP/JU
Sample : K4373-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 26 01:46:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

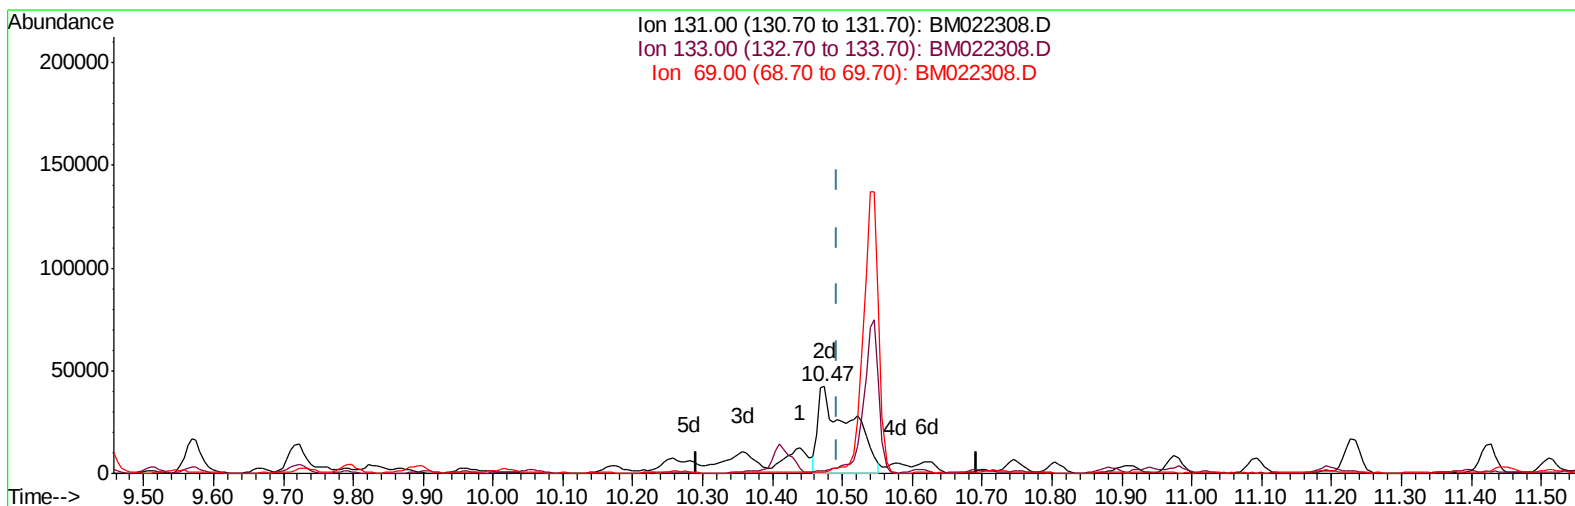

TIC: BM022308.D

(29) 4-Chloroaniline-d4 (S)
10.475min (-0.018) 24.53ng/ul m
response 133783

Ion	Exp%	Act%
131.00	100	100
133.00	31.60	3.46#
69.00	20.00	1.84#
0.00	0.00	0.00