
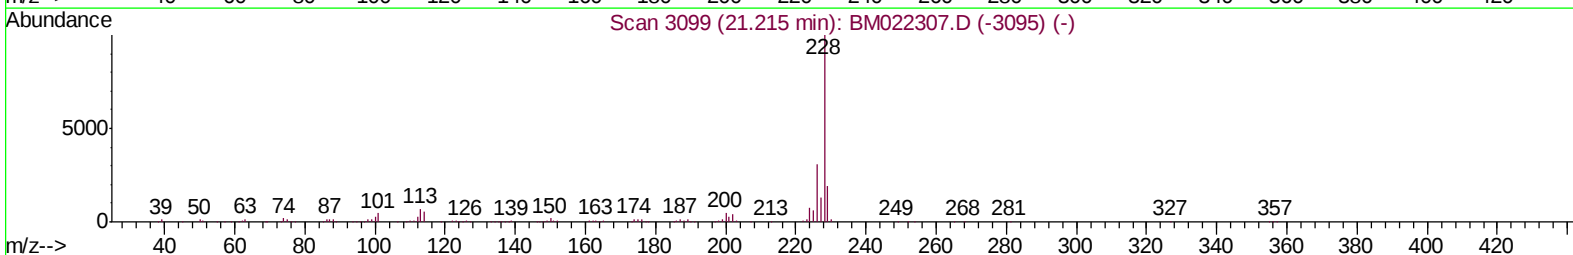
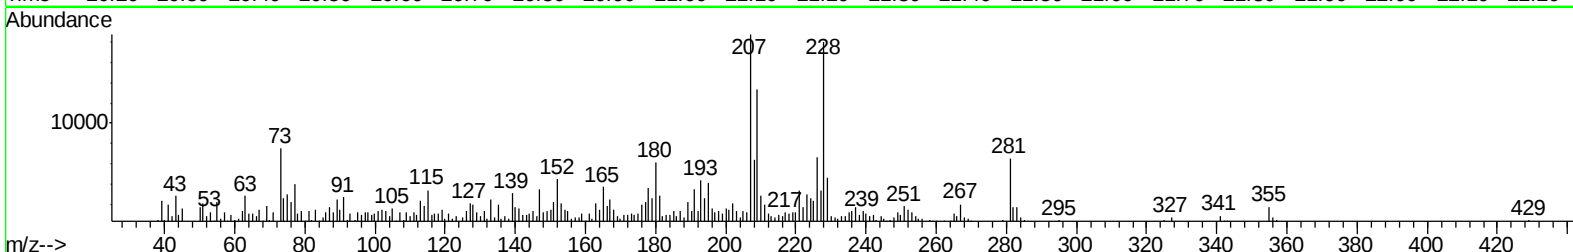


Data File : BM022308.D
Acq On : 25 Aug 2019 01:05
Operator : HP/JU
Sample : K4373-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 26 01:48:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

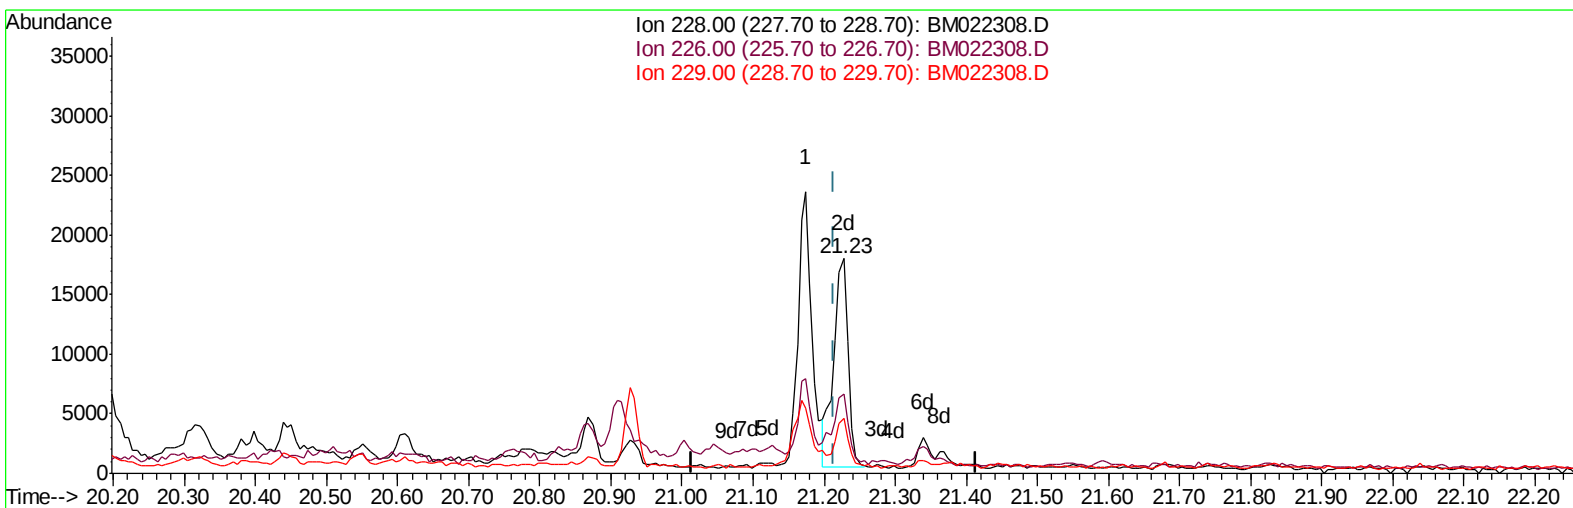

TIC: BM022308.D

(84) Chrysene

21.227min (+0.012) 1.18ng/ul m

response 24563

Ion	Exp%	Act%
228.00	100	100
226.00	30.90	36.92
229.00	19.60	25.81#
0.00	0.00	0.00