
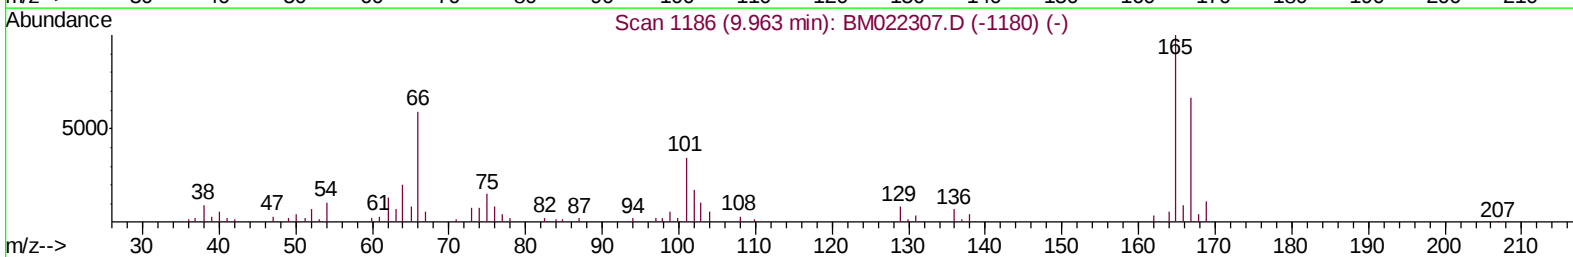
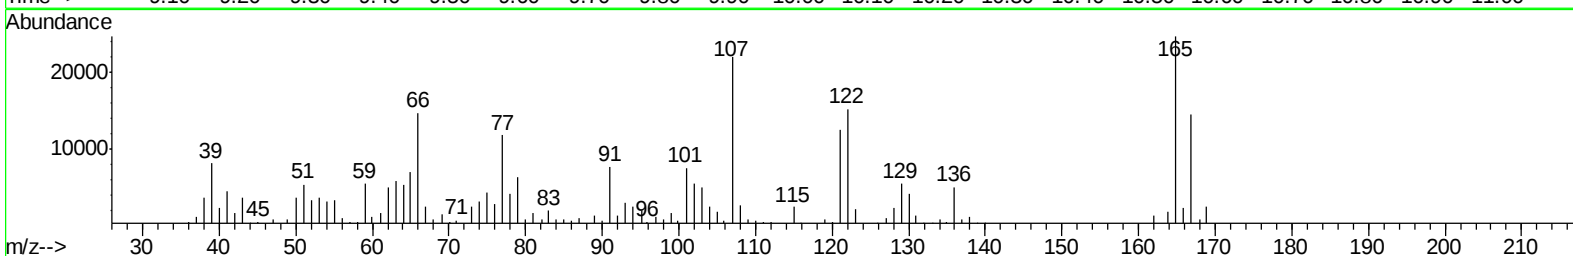


Data File : BM022309.D
Acq On : 25 Aug 2019 01:43
Operator : HP/JU
Sample : K4373-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 26 02:03:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

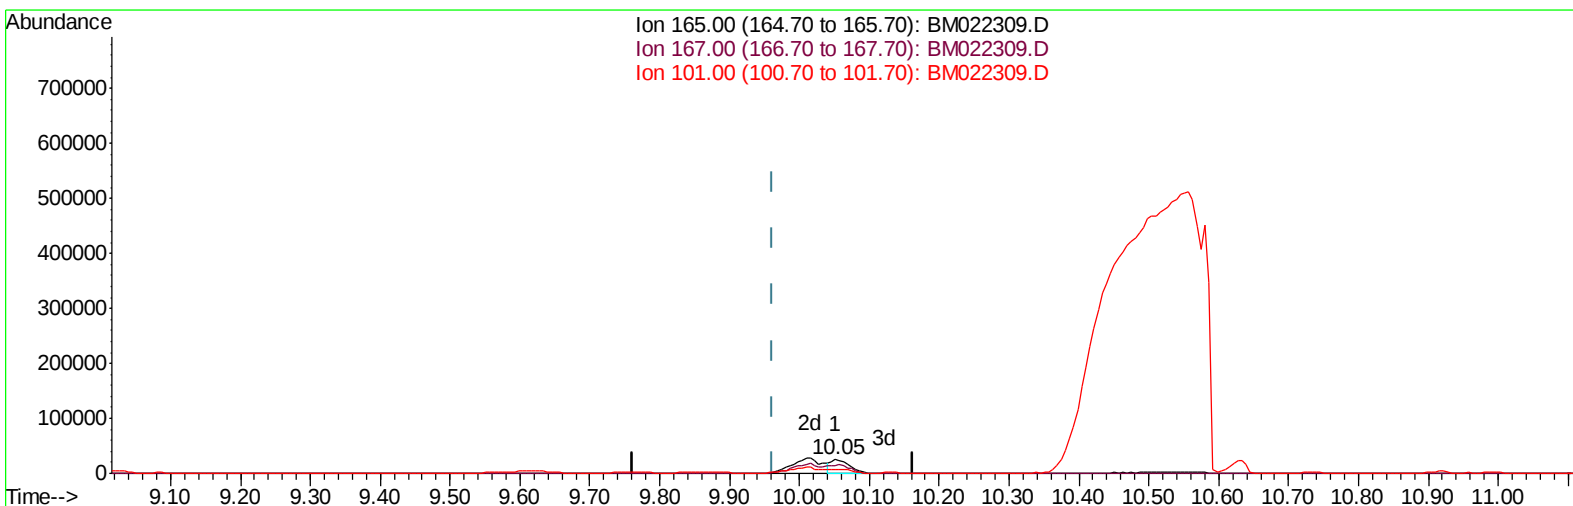

TIC: BM022309.D

(26) 2,4-Dichlorophenol-d3 (S)

10.051min (+0.088) 22.87ng/ul

response 47017

Ion	Exp%	Act%
165.00	100	100
167.00	62.10	58.97
101.00	31.40	30.35
0.00	0.00	0.00