
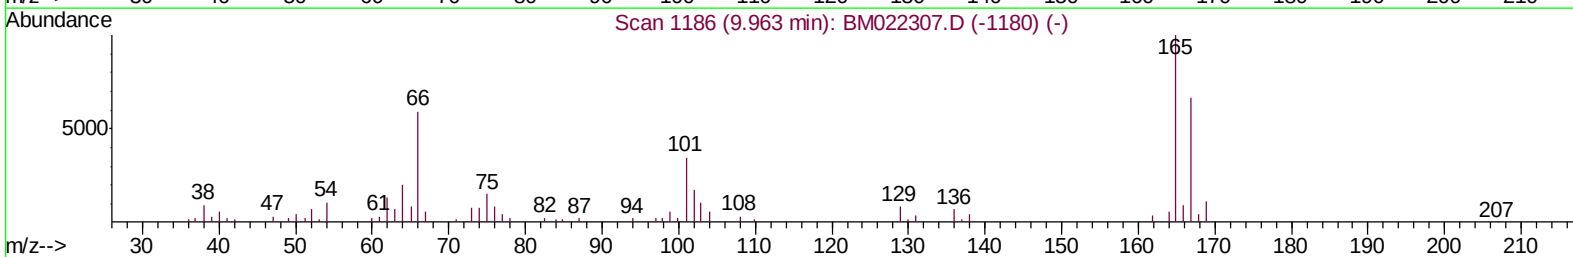
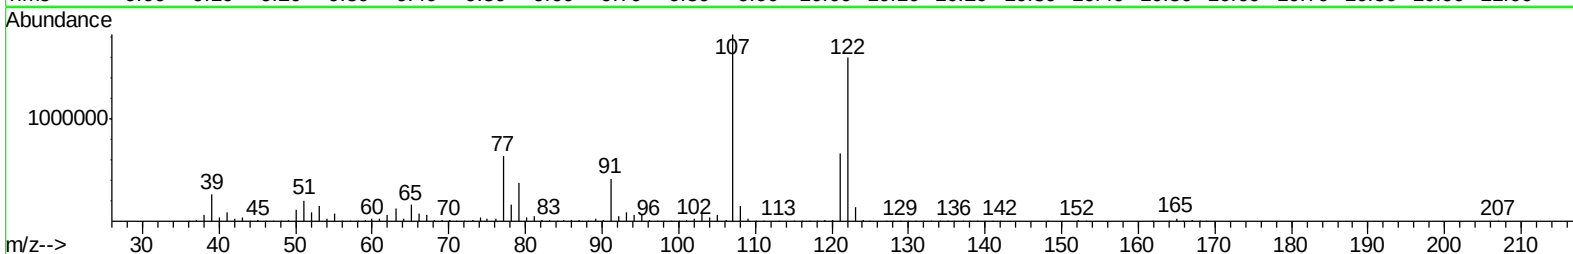


Data File : BM022309.D
Acq On : 25 Aug 2019 01:43
Operator : HP/JU
Sample : K4373-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Aug 26 02:03:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

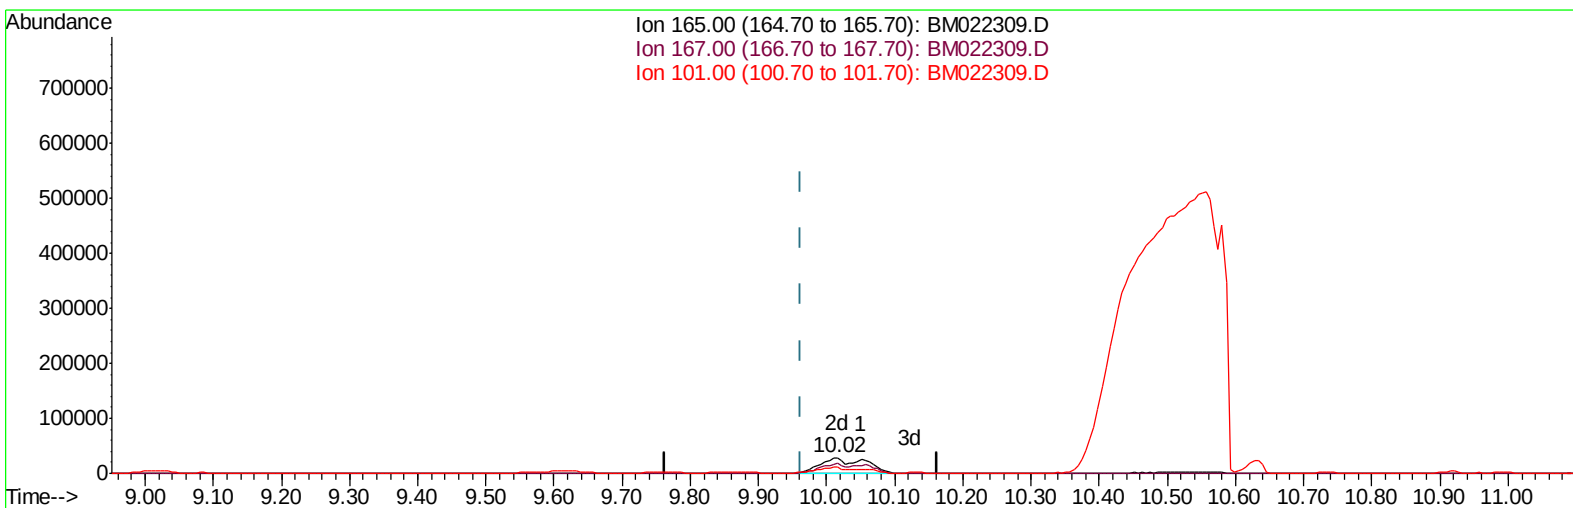

TIC: BM022309.D

(26) 2,4-Dichlorophenol-d3 (S)
10.016min (+0.053) 62.37ng/ul m
response 128223

Ion	Exp%	Act%
165.00	100	100
167.00	62.10	62.97
101.00	31.40	38.71#
0.00	0.00	0.00