
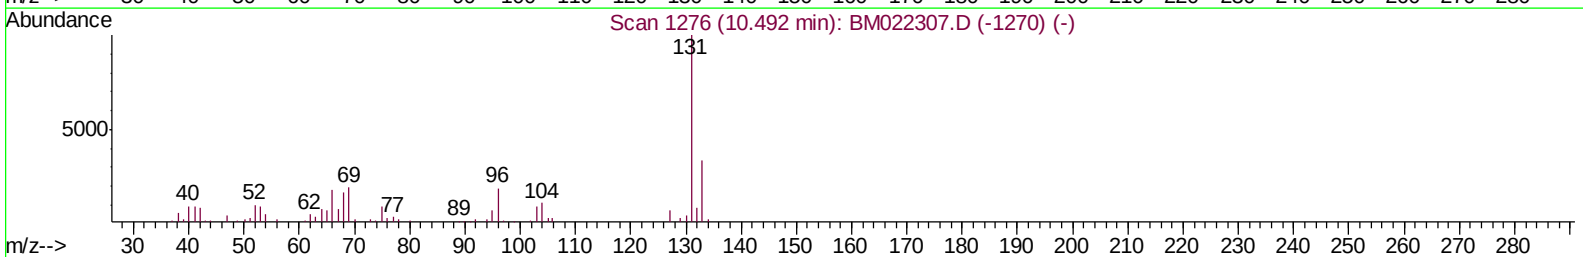
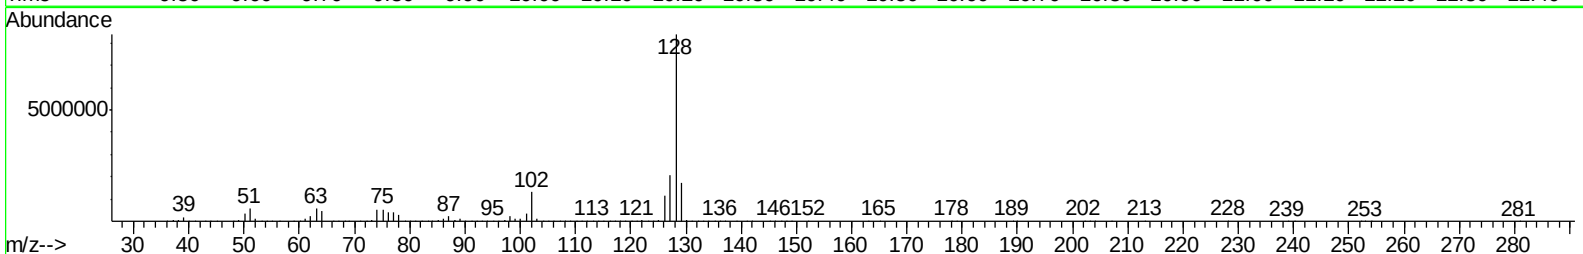


Data File : BM022310.D

```
Acq On       : 25 Aug 2019   02:20
Operator    : HP/JU
Sample      : K4373-19
Misc        :
ALS Vial     : 19      Sample Multip
```

Quant Time: Aug 26 02:31:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

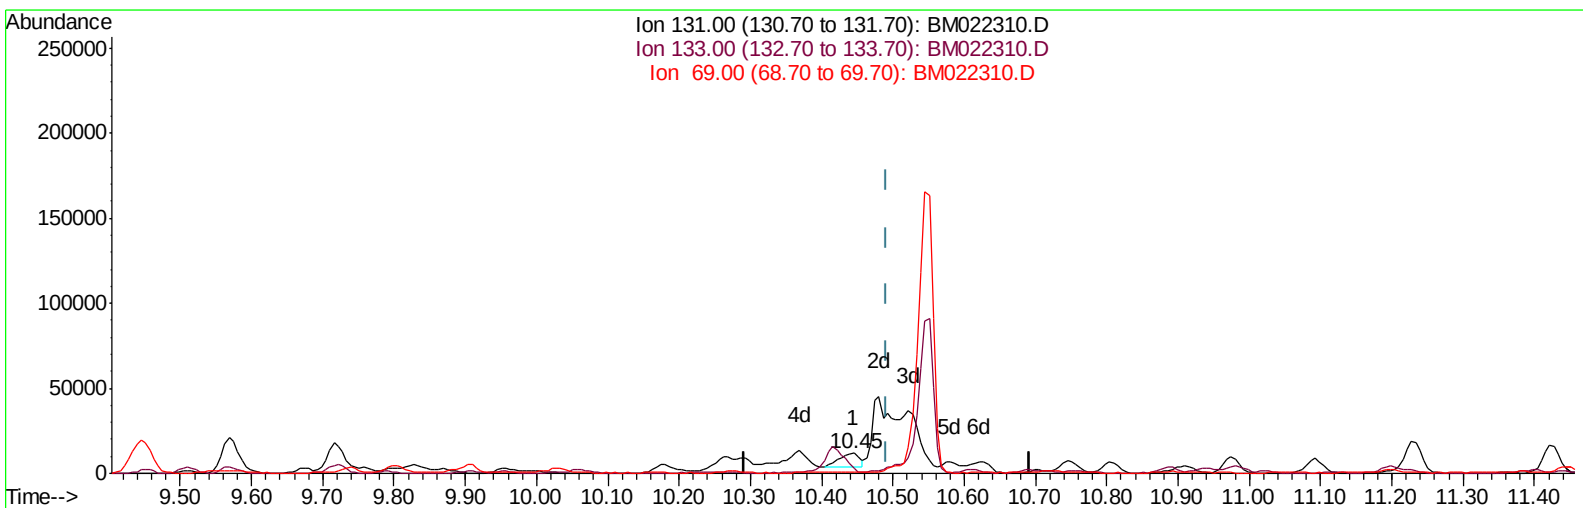

TIC: BM022310.D

(29) 4-Chloroaniline-d4 (S)
10.445min (-0.047) 2.66ng/ul

response 16786

Ion	Exp%	Act%
131.00	100	100
133.00	31.60	24.82#
69.00	20.00	5.35#
0.00	0.00	0.00