
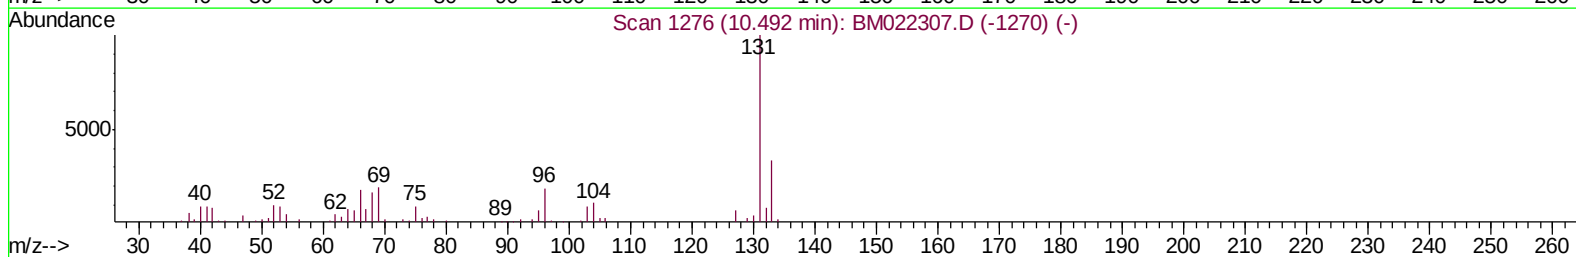
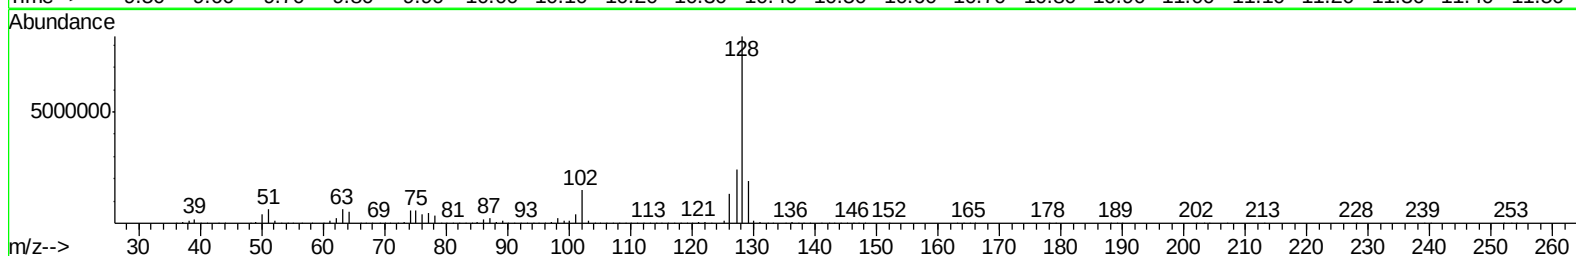


Data File : BM022310.D
Acq On : 25 Aug 2019 02:20
Operator : HP/JU
Sample : K4373-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 26 02:31:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

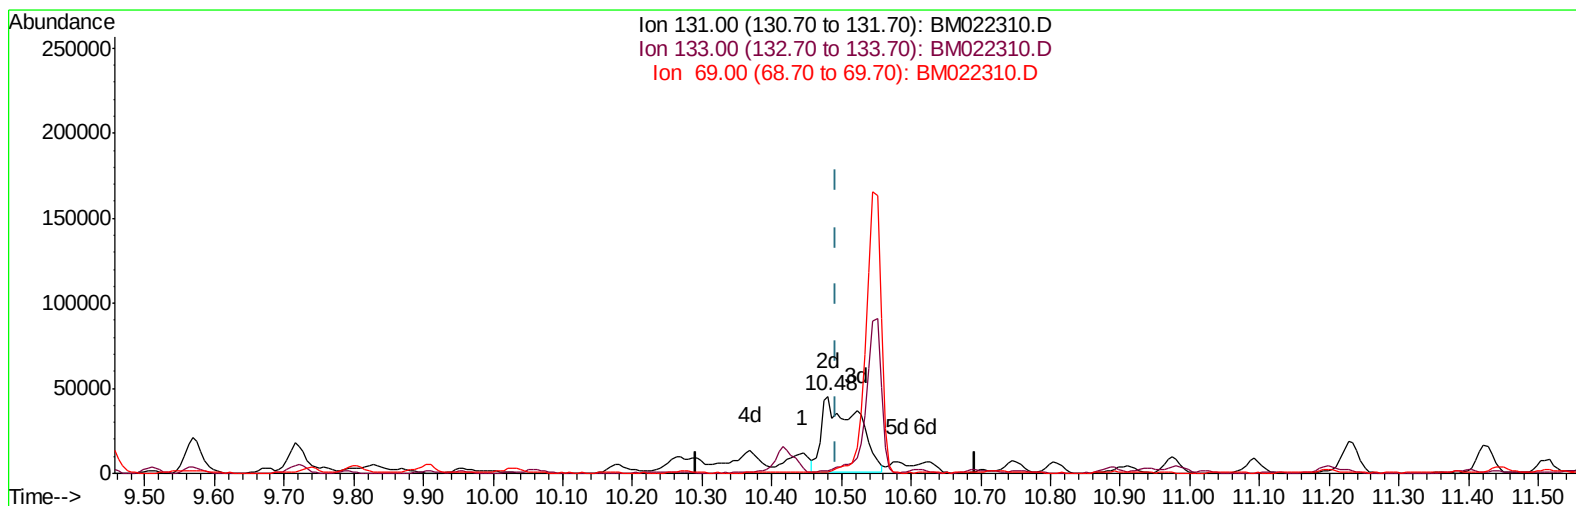

TIC: BM022310.D

(29) 4-Chloroaniline-d4 (S)
10.480min (-0.012) 24.48ng/ul m
response 154564

Ion	Exp%	Act%
131.00	100	100
133.00	31.60	3.83#
69.00	20.00	2.17#
0.00	0.00	0.00