
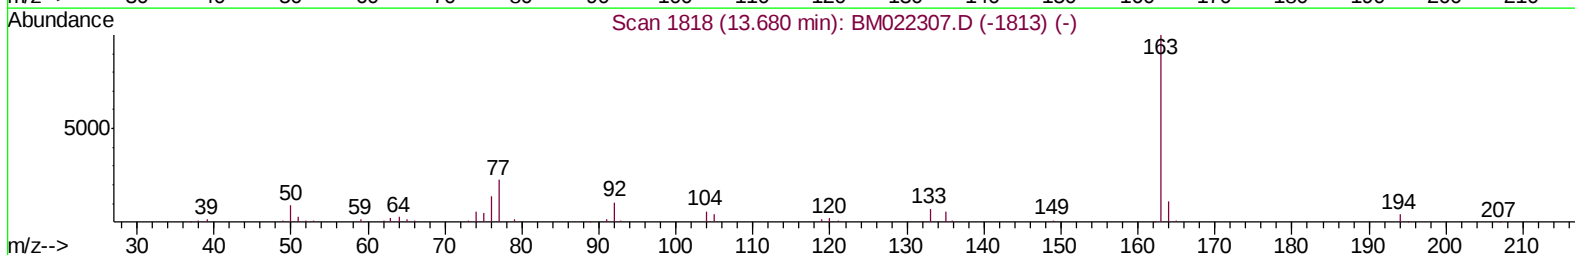
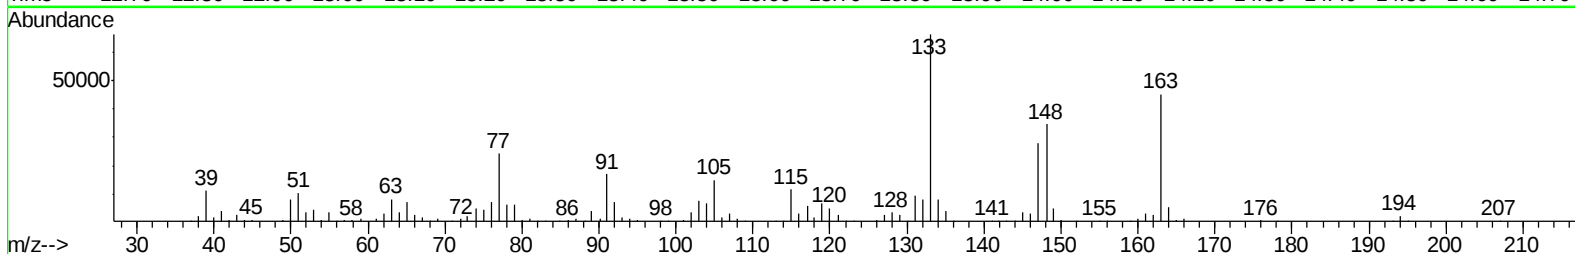


Data File : BM022308.D
Acq On : 25 Aug 2019 01:05
Operator : HP/JU
Sample : K4373-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 26 01:53:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

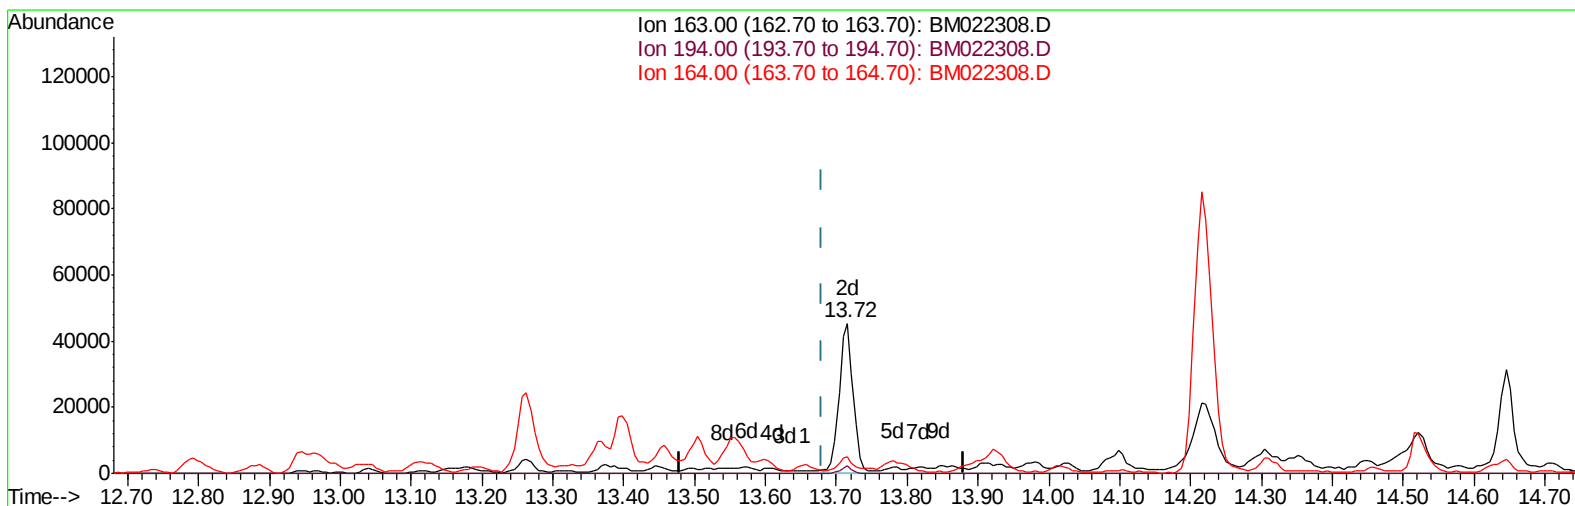

TIC: BM022308.D

(44) Dimethylphthalate

13.716min (+0.035) 4.56ng/ul m

response 62420

Ion	Exp%	Act%
163.00	100	100
194.00	3.80	4.74#
164.00	9.80	11.46
0.00	0.00	0.00