
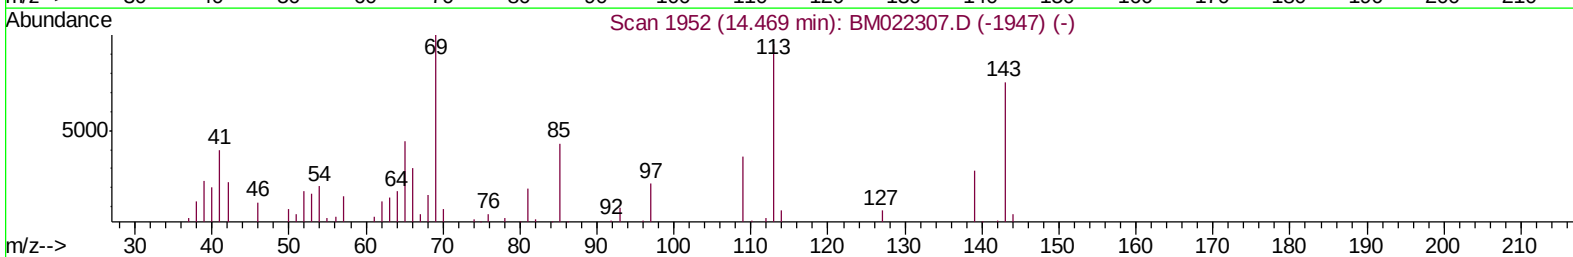
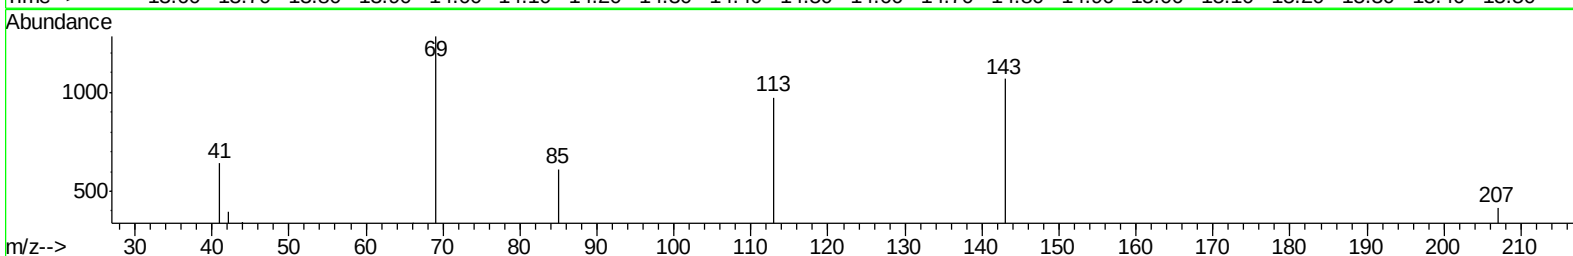


Data File : BM022315.D
Acq On : 25 Aug 2019 05:25
Operator : HP/JU
Sample : K4373-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Aug 26 01:37:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

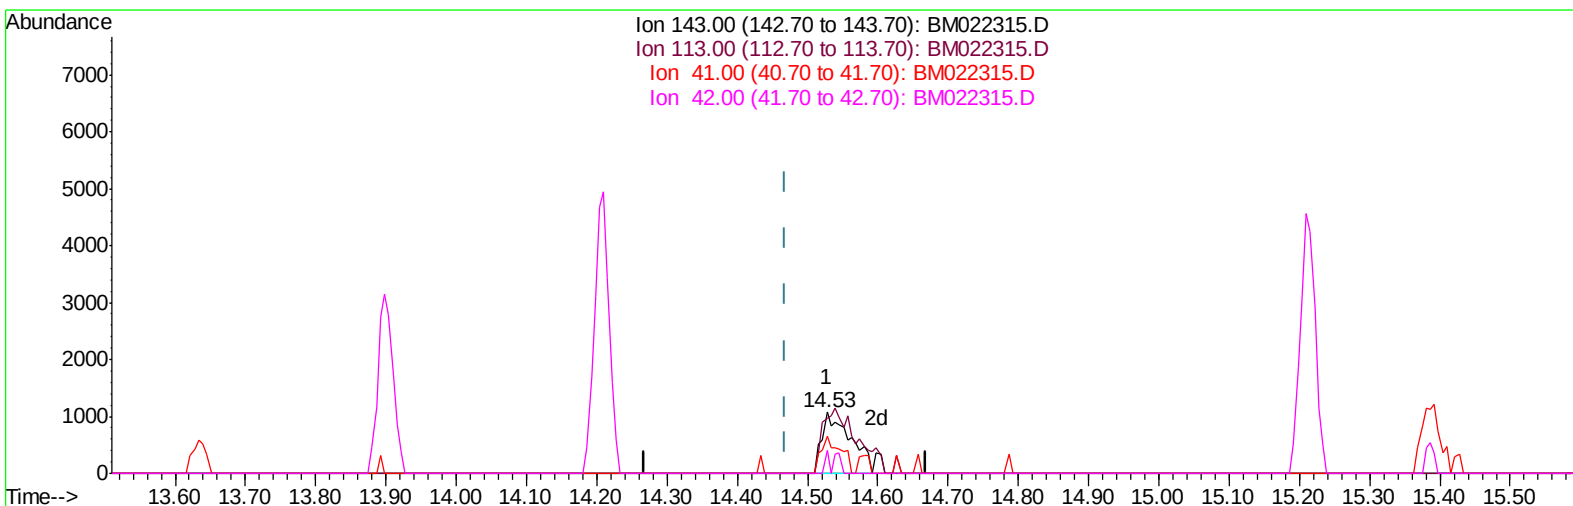

TIC: BM022315.D

(51) 4-Nitrophenol-d4 (S)

14.527min (+0.059) 1.90ng/ul m

response 3020

Ion	Exp%	Act%
143.00	100	100
113.00	116.00	91.12#
41.00	50.80	60.00
42.00	27.00	37.10#