
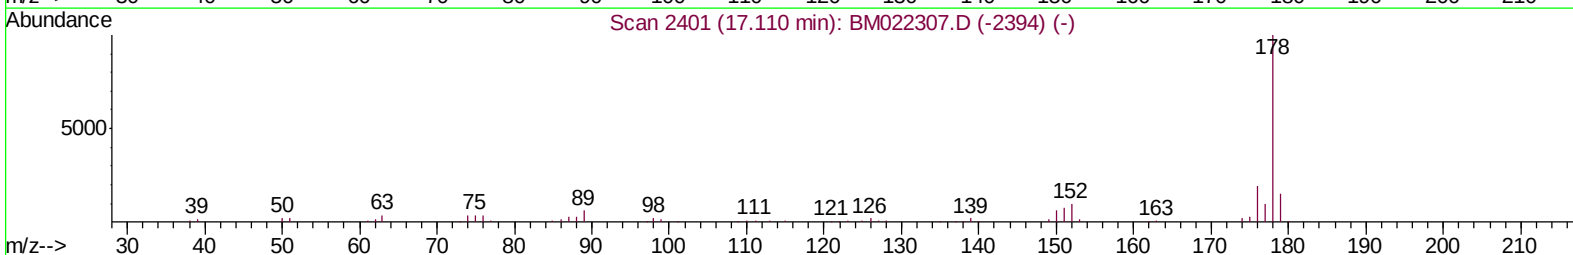
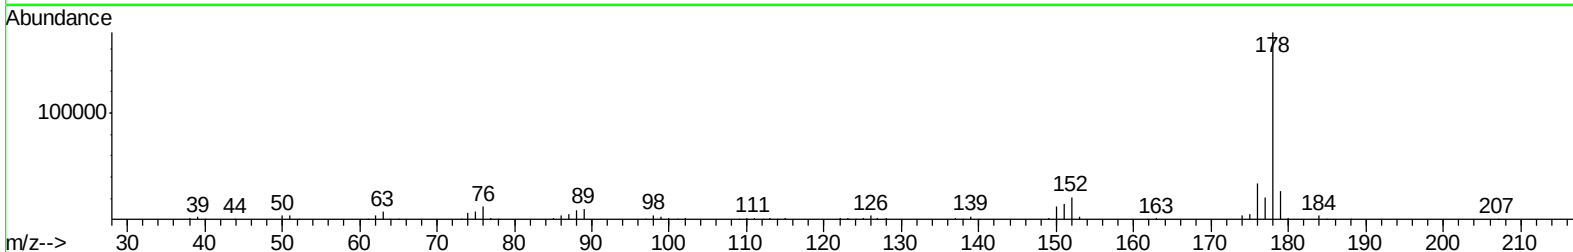


Data File : BM022316.D
Acq On : 25 Aug 2019 06:01
Operator : HP/JU
Sample : K4242-02ME
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Aug 26 01:37:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

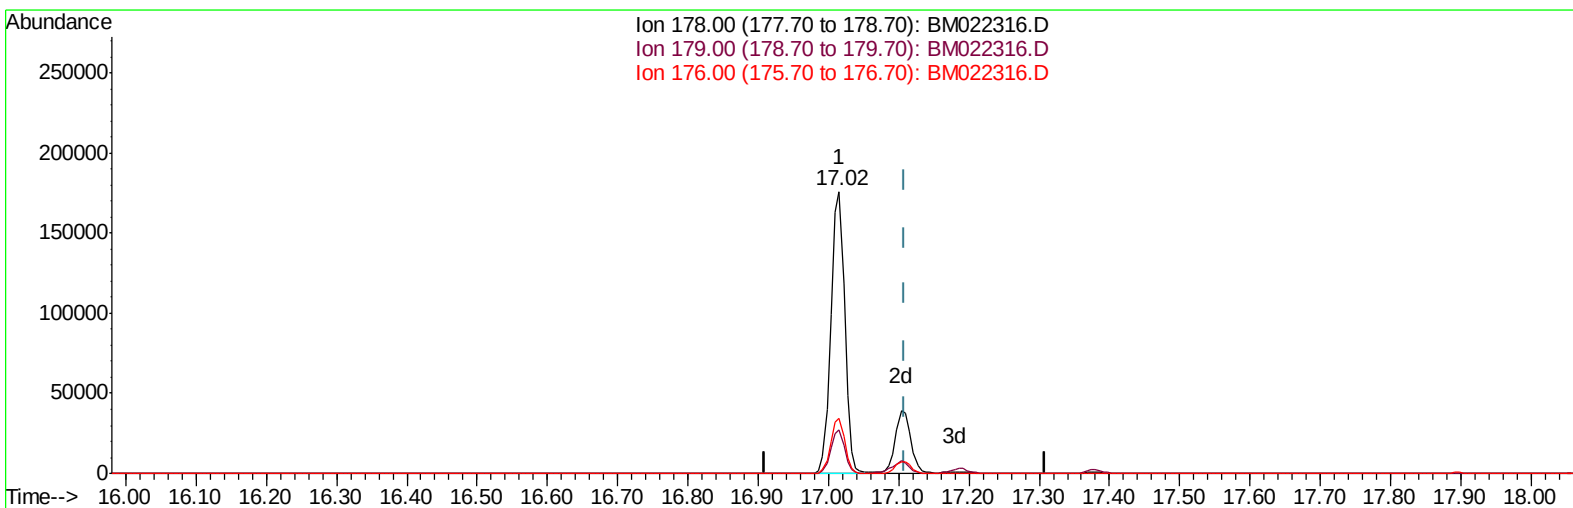

TIC: BM022316.D

(71) Anthracene

17.015min (-0.094) 14.32ng/ul

response 238338

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.38
176.00	19.40	19.66
0.00	0.00	0.00