
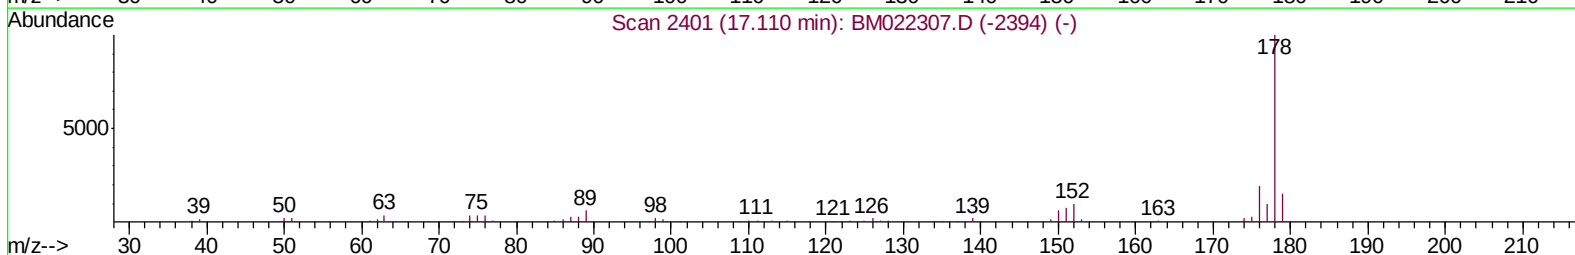
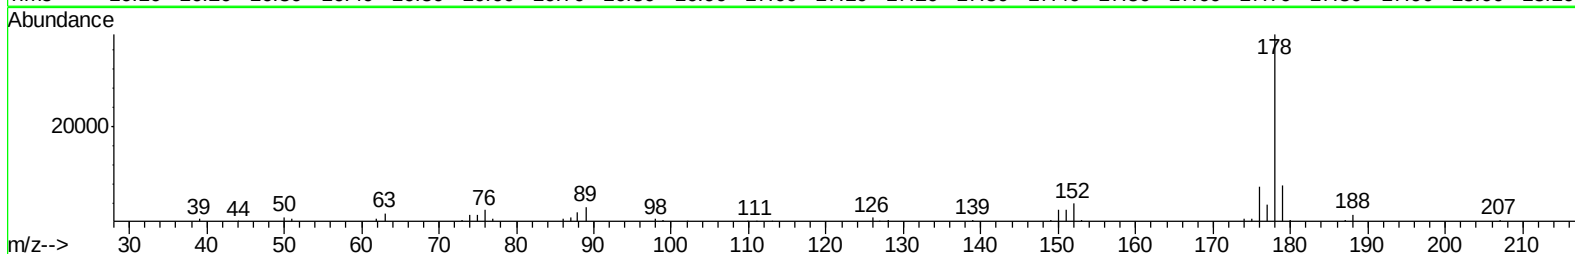


Data File : BM022316.D  
Acq On : 25 Aug 2019 06:01  
Operator : HP/JU  
Sample : K4242-02ME  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Aug 26 01:37:08 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM082219MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Aug 26 01:32:10 2019  
Response via : Initial Calibration

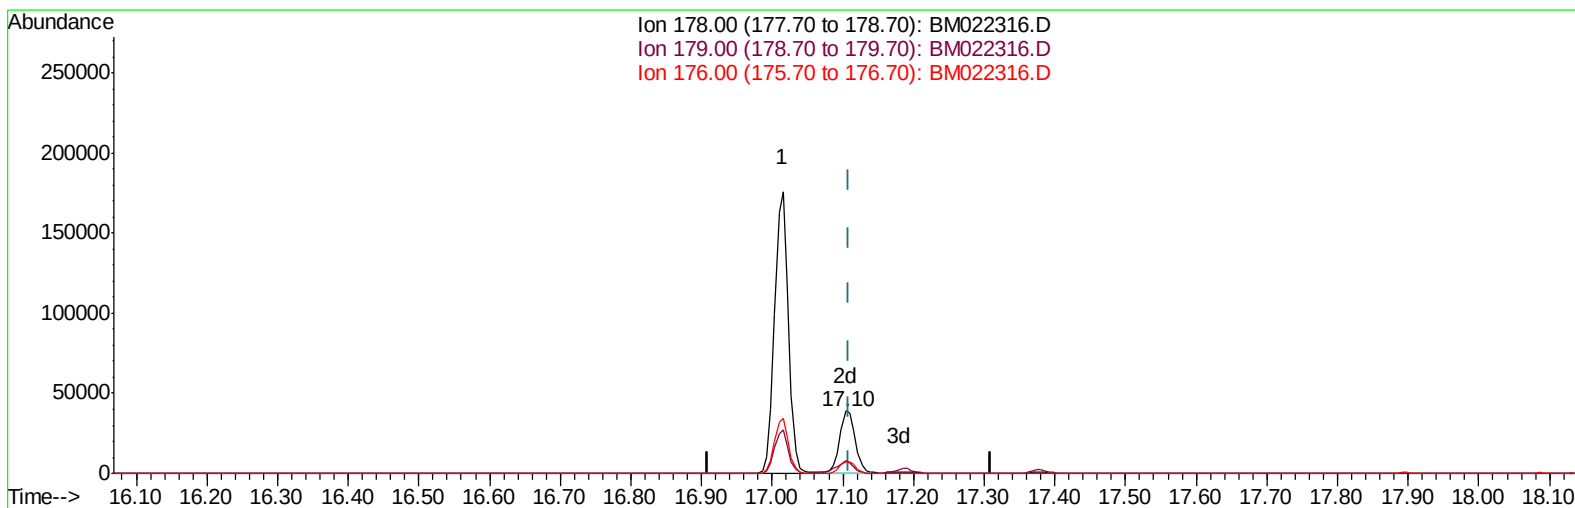

TIC: BM022316.D

(71) Anthracene

17.104min (-0.006) 3.56ng/ul m

response 59248

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 178.00 | 100   | 100    |
| 179.00 | 15.40 | 19.56# |
| 176.00 | 19.40 | 19.08  |
| 0.00   | 0.00  | 0.00   |