
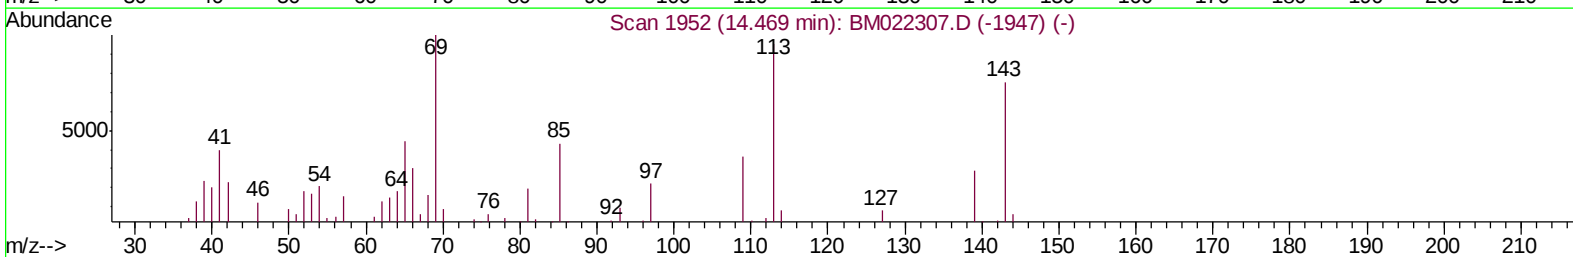
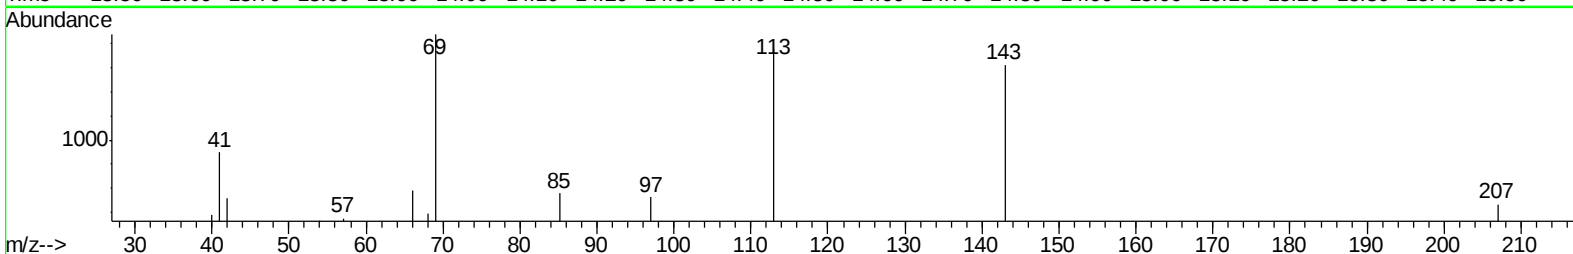


Data File : BM022320.D
Acq On : 25 Aug 2019 08:27
Operator : HP/JU
Sample : K4373-21
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Aug 26 01:37:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

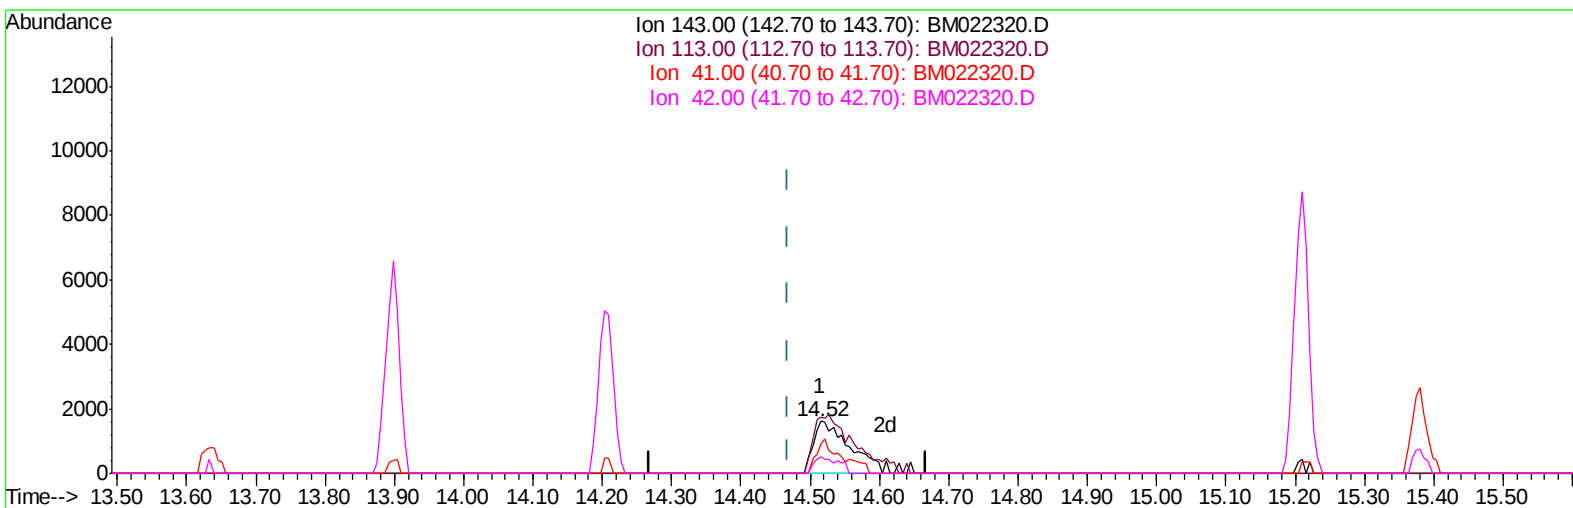

TIC: BM022320.D

(51) 4-Nitrophenol-d4 (S)

14.515min (+0.047) 3.23ng/ul m

response 5815

Ion	Exp%	Act%
143.00	100	100
113.00	116.00	108.78
41.00	50.80	55.47
42.00	27.00	31.97