
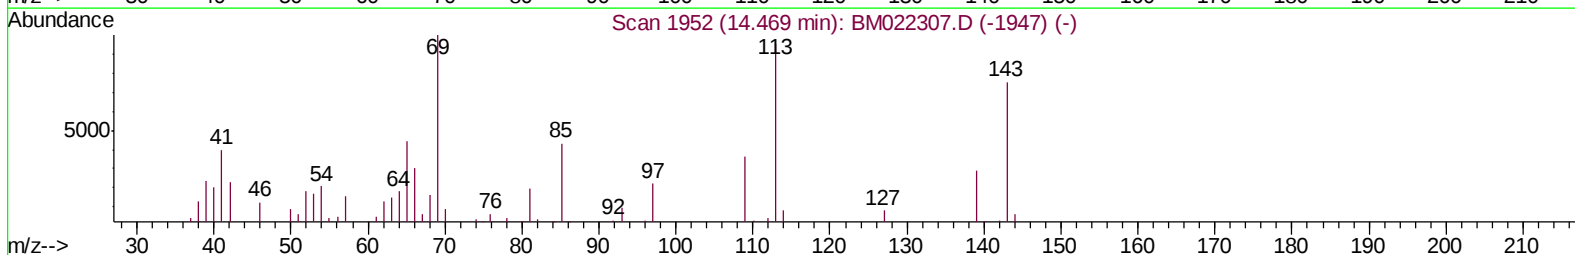
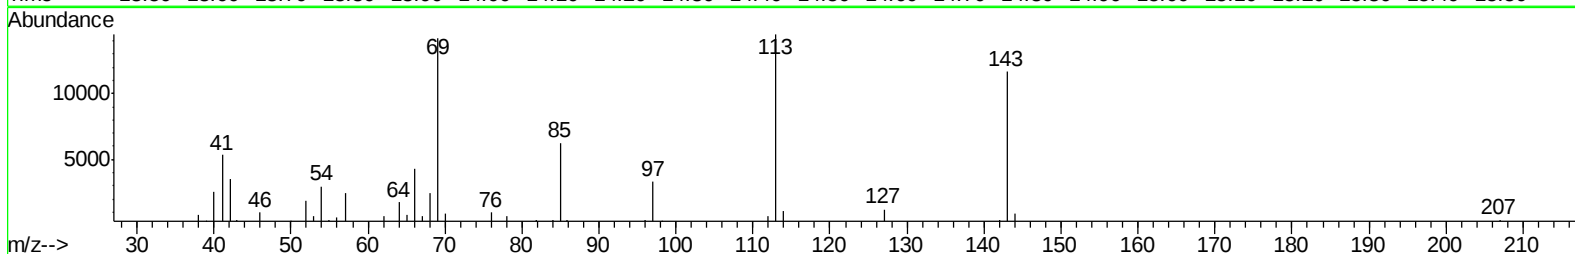


Data File : BM022321.D
Acq On : 25 Aug 2019 09:04
Operator : HP/JU
Sample : PB122530BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 26 01:37:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

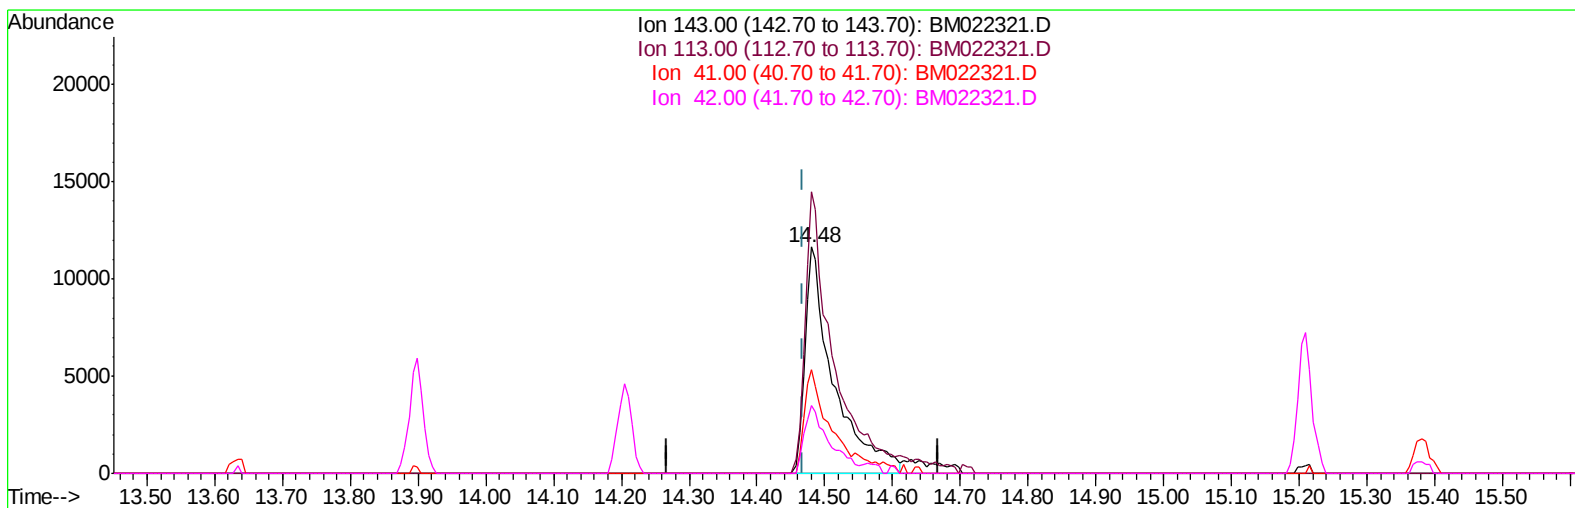

TIC: BM022321.D

(51) 4-Nitrophenol-d4 (S)

14.480min (+0.012) 23.22ng/ul m

response 34139

Ion	Exp%	Act%
143.00	100	100
113.00	116.00	124.53
41.00	50.80	45.86
42.00	27.00	30.23