
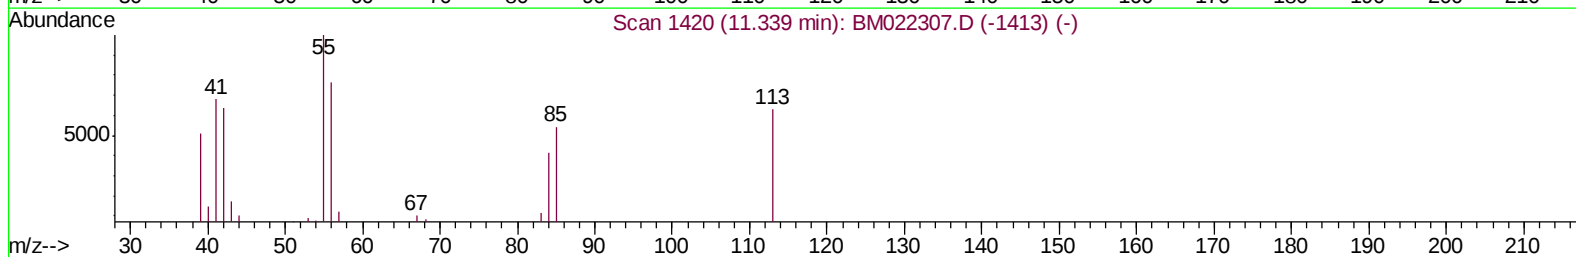
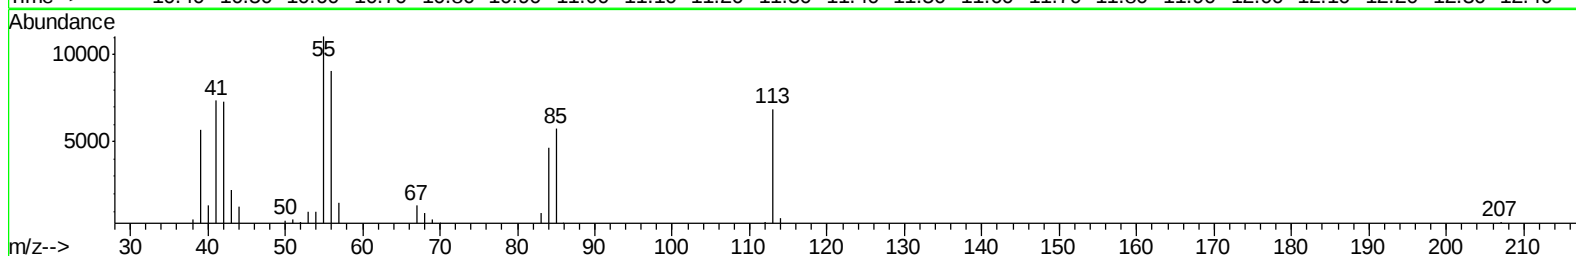


Data File : BM022322.D
Acq On : 25 Aug 2019 10:54
Operator : HP/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Aug 26 01:37:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 26 01:32:10 2019
Response via : Initial Calibration

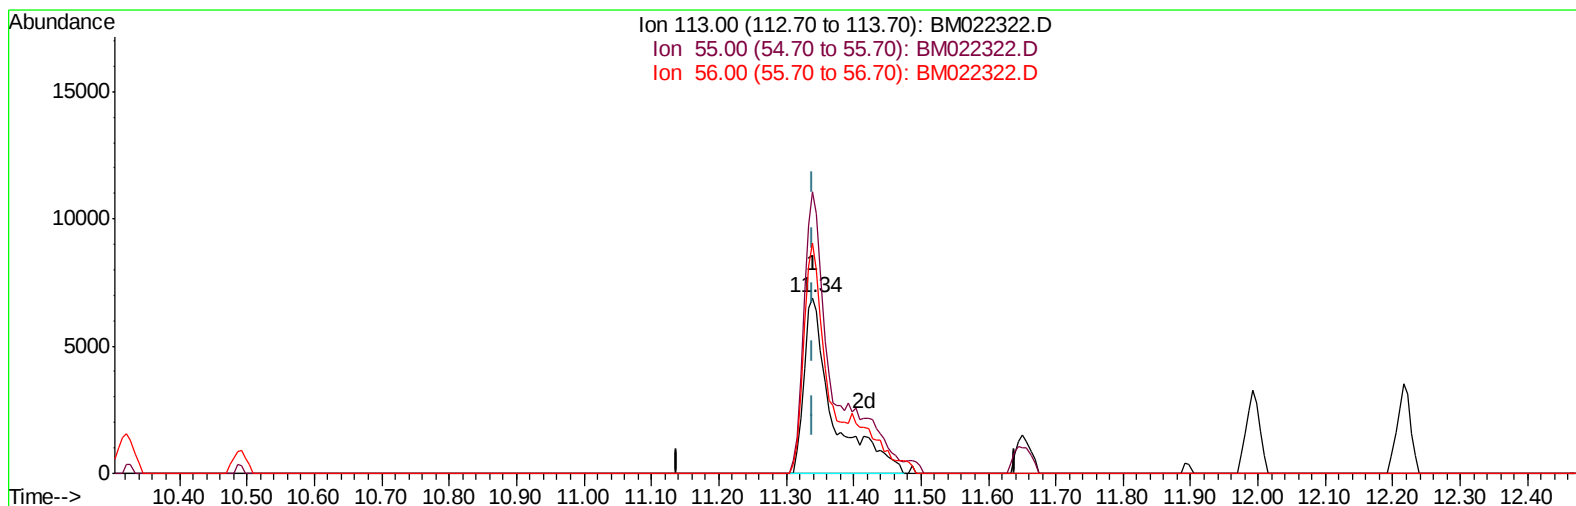

TIC: BM022322.D

(32) Caprolactam

11.339min (-0.000) 22.55ng/ul m

response 20508

Ion	Exp%	Act%
113.00	100	100
55.00	139.50	160.40
56.00	130.80	131.19
0.00	0.00	0.00