

Data File : BM022274.D
Acq On : 24 Aug 2019 02:15
Operator : HP/JU
Sample : PB122304BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK04

Quant Time: Aug 24 05:41:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 24 01:09:04 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	26391	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	117752	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	82064	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	192862	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	231565	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	238755	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	3801	6.45	ng/uL	0.00
5) Phenol-d5	6.75	99	63412	27.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	41219	31.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	56171	30.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	56308	28.52	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	28284	32.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	32398	31.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	58458	28.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	84509	33.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	241294	33.39	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	267608	34.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	23528	21.98	ng/ul	0.00
57) Fluorene-d10	15.22	176	200207	33.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	32240	21.66	ng/ul	0.00
70) Anthracene-d10	17.07	188	332684	32.58	ng/ul	0.00
78) Pyrene-d10	19.38	212	464610	38.61	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	439587	33.51	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.28	70	1730	1.001	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM022274.D
Acq On : 24 Aug 2019 02:15
Operator : HP/JU
Sample : PB122304BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK04

Quant Time: Aug 24 05:41:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 24 01:09:04 2019
Response via : Initial Calibration

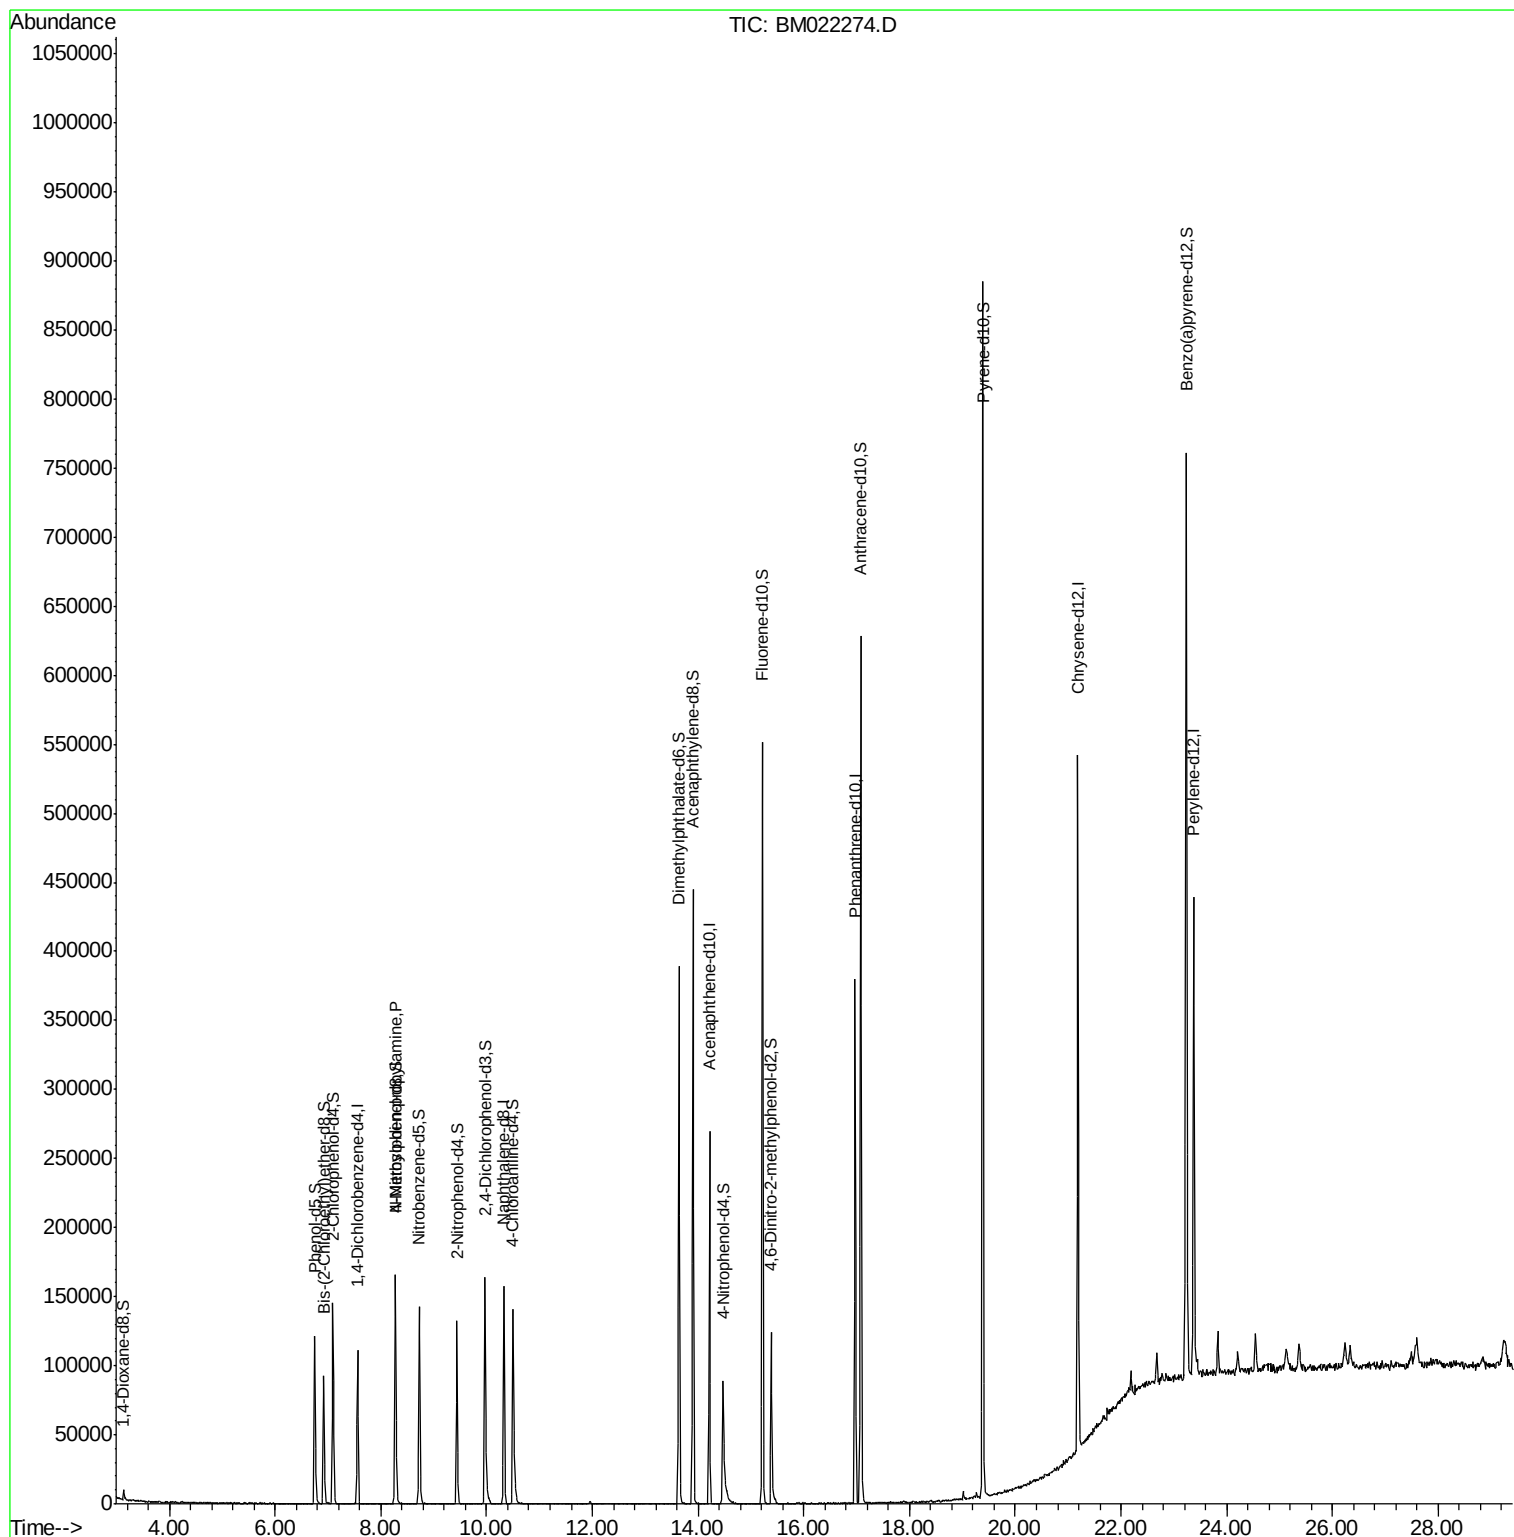

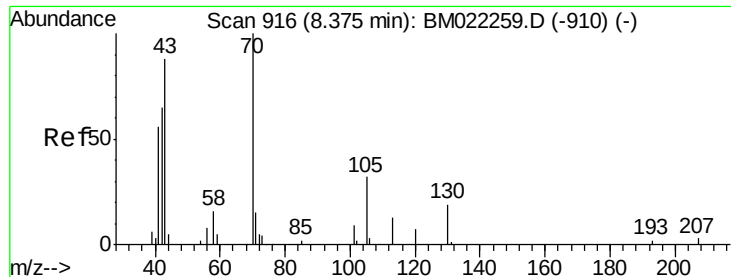

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.001 ng/ul
 RT: 8.28 min Scan# 900
 Delta R.T. -0.09 min
 Lab File: BM022274.D
 Acq: 24 Aug 2019 02:15

Instrument :
 BNA_M
 ClientSampleId :
 SBLK04

Tgt Ion:	70	Resp:	1730
Ion	Ratio	Lower	Upper
70	100		
42	360.1	55.1	82.7#
101	0.0	8.0	12.0#
130	0.0	15.7	23.5#

