

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
 Data File : BM022281.D
 Acq On : 24 Aug 2019 06:37
 Operator : HP/JU
 Sample : PB122266BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK66

Quant Time: Aug 25 01:23:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 25 01:20:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	33011	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	147373	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	102431	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	236675	20.00	ng/ul	0.00
77) Chrysene-d12	21.18	240	282575	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	271608	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	3986	5.40	ng/uL	0.00
5) Phenol-d5	6.75	99	77249	27.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	47472	28.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	67085	29.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	69109	27.99	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	33815	30.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	39136	30.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	74976	28.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	98319	31.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	273810	30.35	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	316429	32.57	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	32710	24.48	ng/ul	0.00
57) Fluorene-d10	15.22	176	231450	30.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	36805	20.15	ng/ul	0.00
70) Anthracene-d10	17.07	188	382112	30.49	ng/ul	0.00
78) Pyrene-d10	19.38	212	526317	35.84	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	464296	31.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.27	70	2221	1.028	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022281.D
Acq On : 24 Aug 2019 06:37
Operator : HP/JU
Sample : PB122266BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Time: Aug 25 01:23:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 25 01:20:09 2019
Response via : Initial Calibration

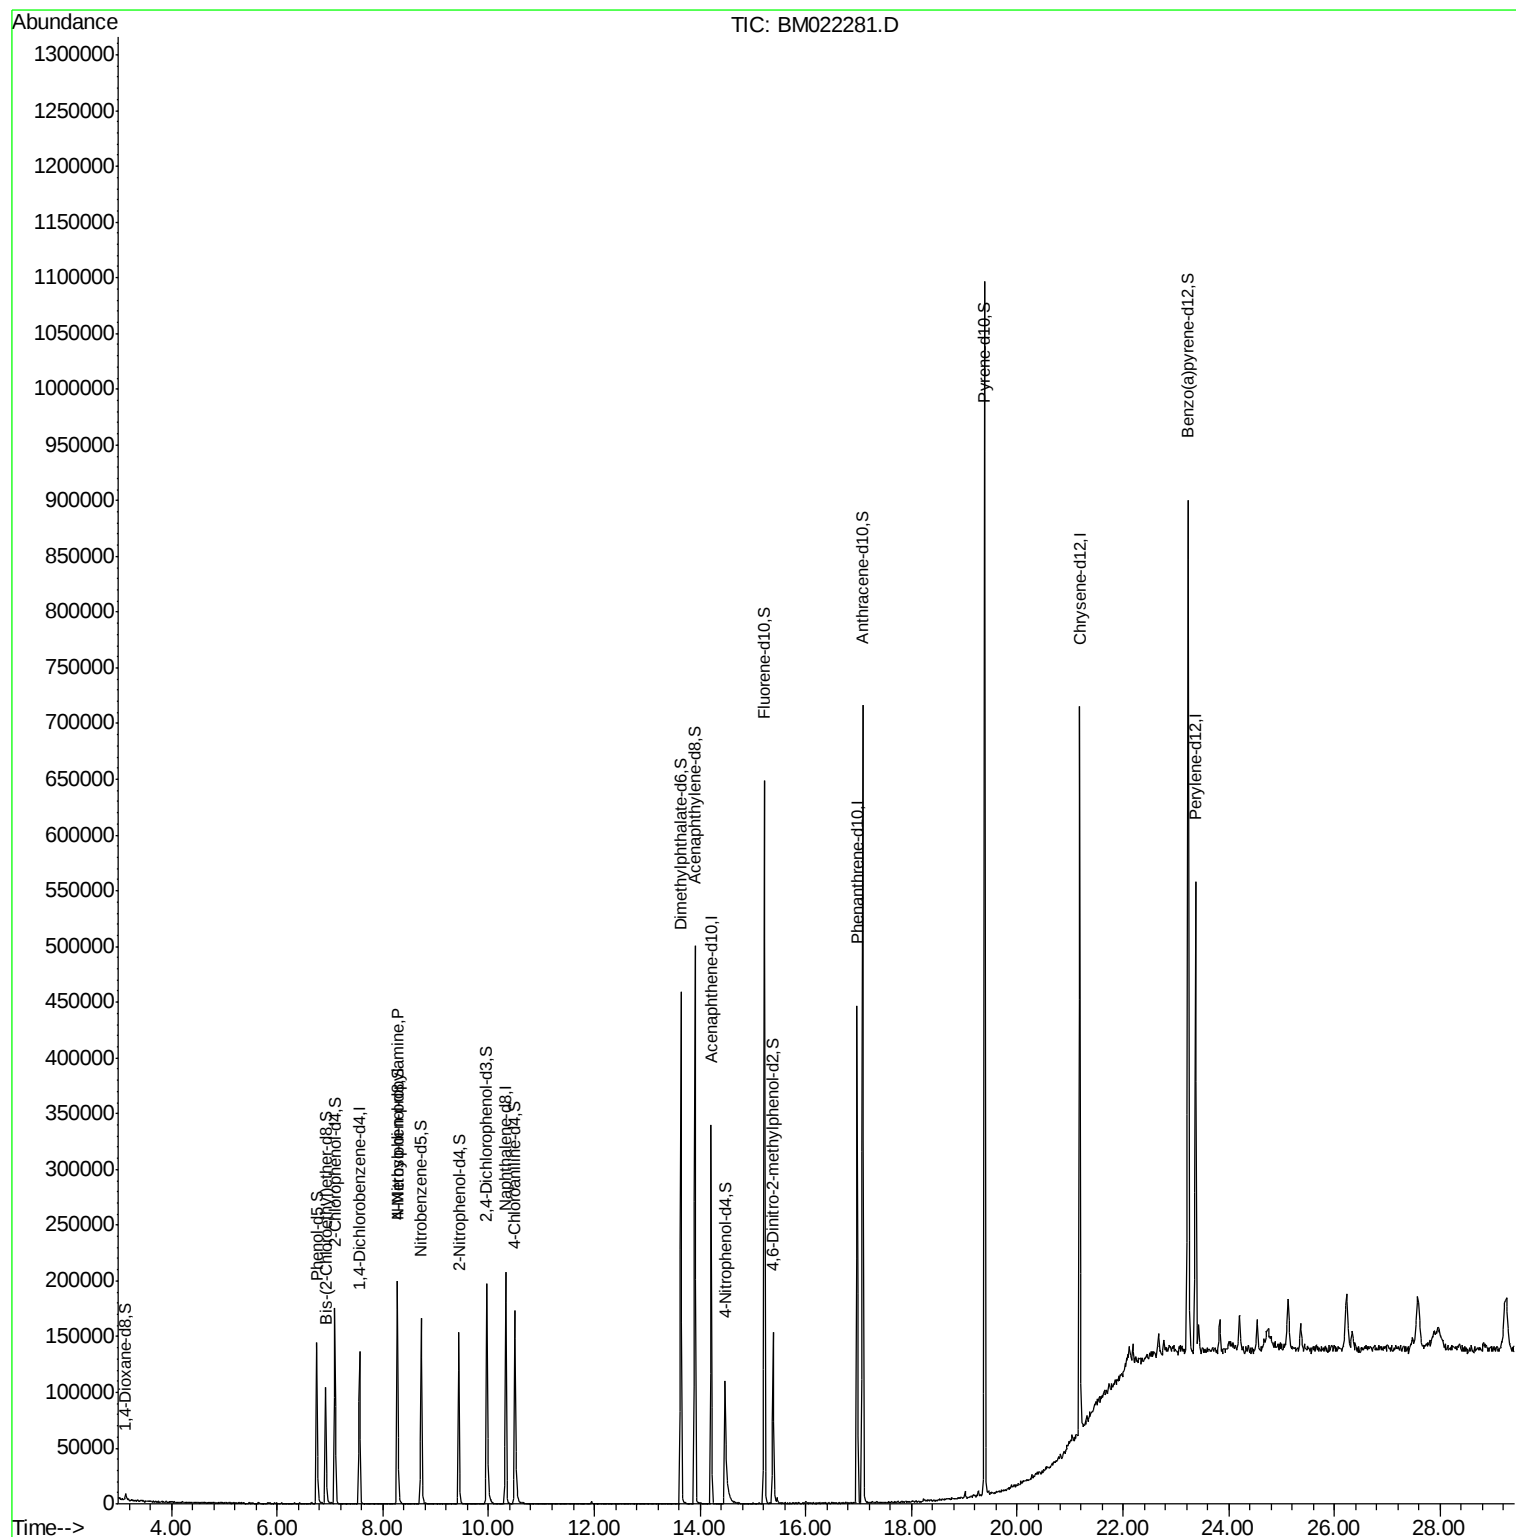

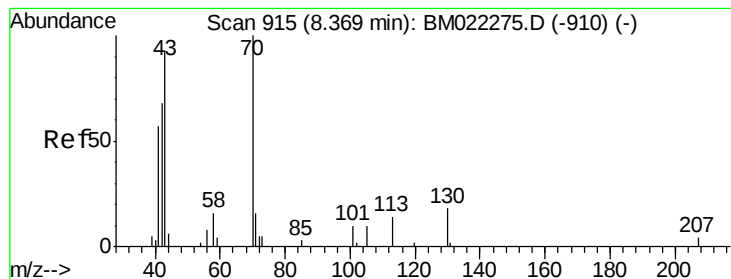

#15

N-Nitroso-di-n-propylamine

Concen: 1.028 ng/ul

RT: 8.27 min Scan# 899

Delta R.T. -0.09 min

Lab File: BM022281.D


Acq: 24 Aug 2019 06:37

Instrument :

BNA_M

ClientSampleId :

SBLK66

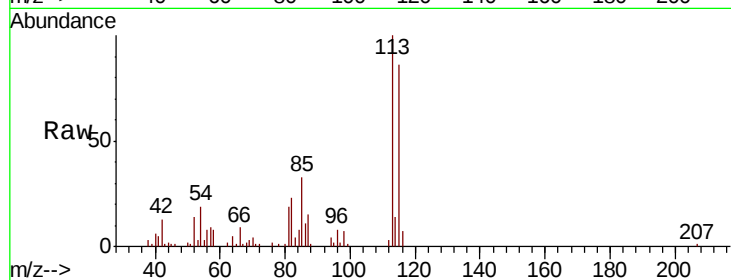

Tgt Ion: 70 Resp: 2221


Ion Ratio Lower Upper

70 100

42 353.2 55.1 82.7#

101 0.0 8.0 12.0#

130 0.0 15.7 23.5#

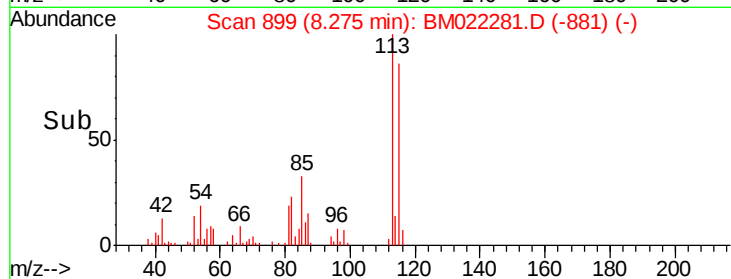

Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

