

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
 Data File : BM022283.D
 Acq On : 24 Aug 2019 07:51
 Operator : HP/JU
 Sample : PB122365BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Aug 25 01:23:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 25 01:20:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	36059	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	161101	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	112128	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	257429	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	273461	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	244009	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	4772	5.92	ng/uL	0.00
5) Phenol-d5	6.75	99	86277	27.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	53657	29.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	75536	30.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	77370	28.69	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	38031	31.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	44507	31.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	82842	29.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	114333	33.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	313873	31.79	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	359666	33.82	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	34706	23.73	ng/ul	0.00
57) Fluorene-d10	15.22	176	265086	32.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	42536	21.41	ng/ul	0.00
70) Anthracene-d10	17.07	188	431755	31.67	ng/ul	0.00
78) Pyrene-d10	19.38	212	578818	40.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	435064	32.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.27	70	2462	1.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022283.D
Acq On : 24 Aug 2019 07:51
Operator : HP/JU
Sample : PB122365BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Time: Aug 25 01:23:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 25 01:20:09 2019
Response via : Initial Calibration

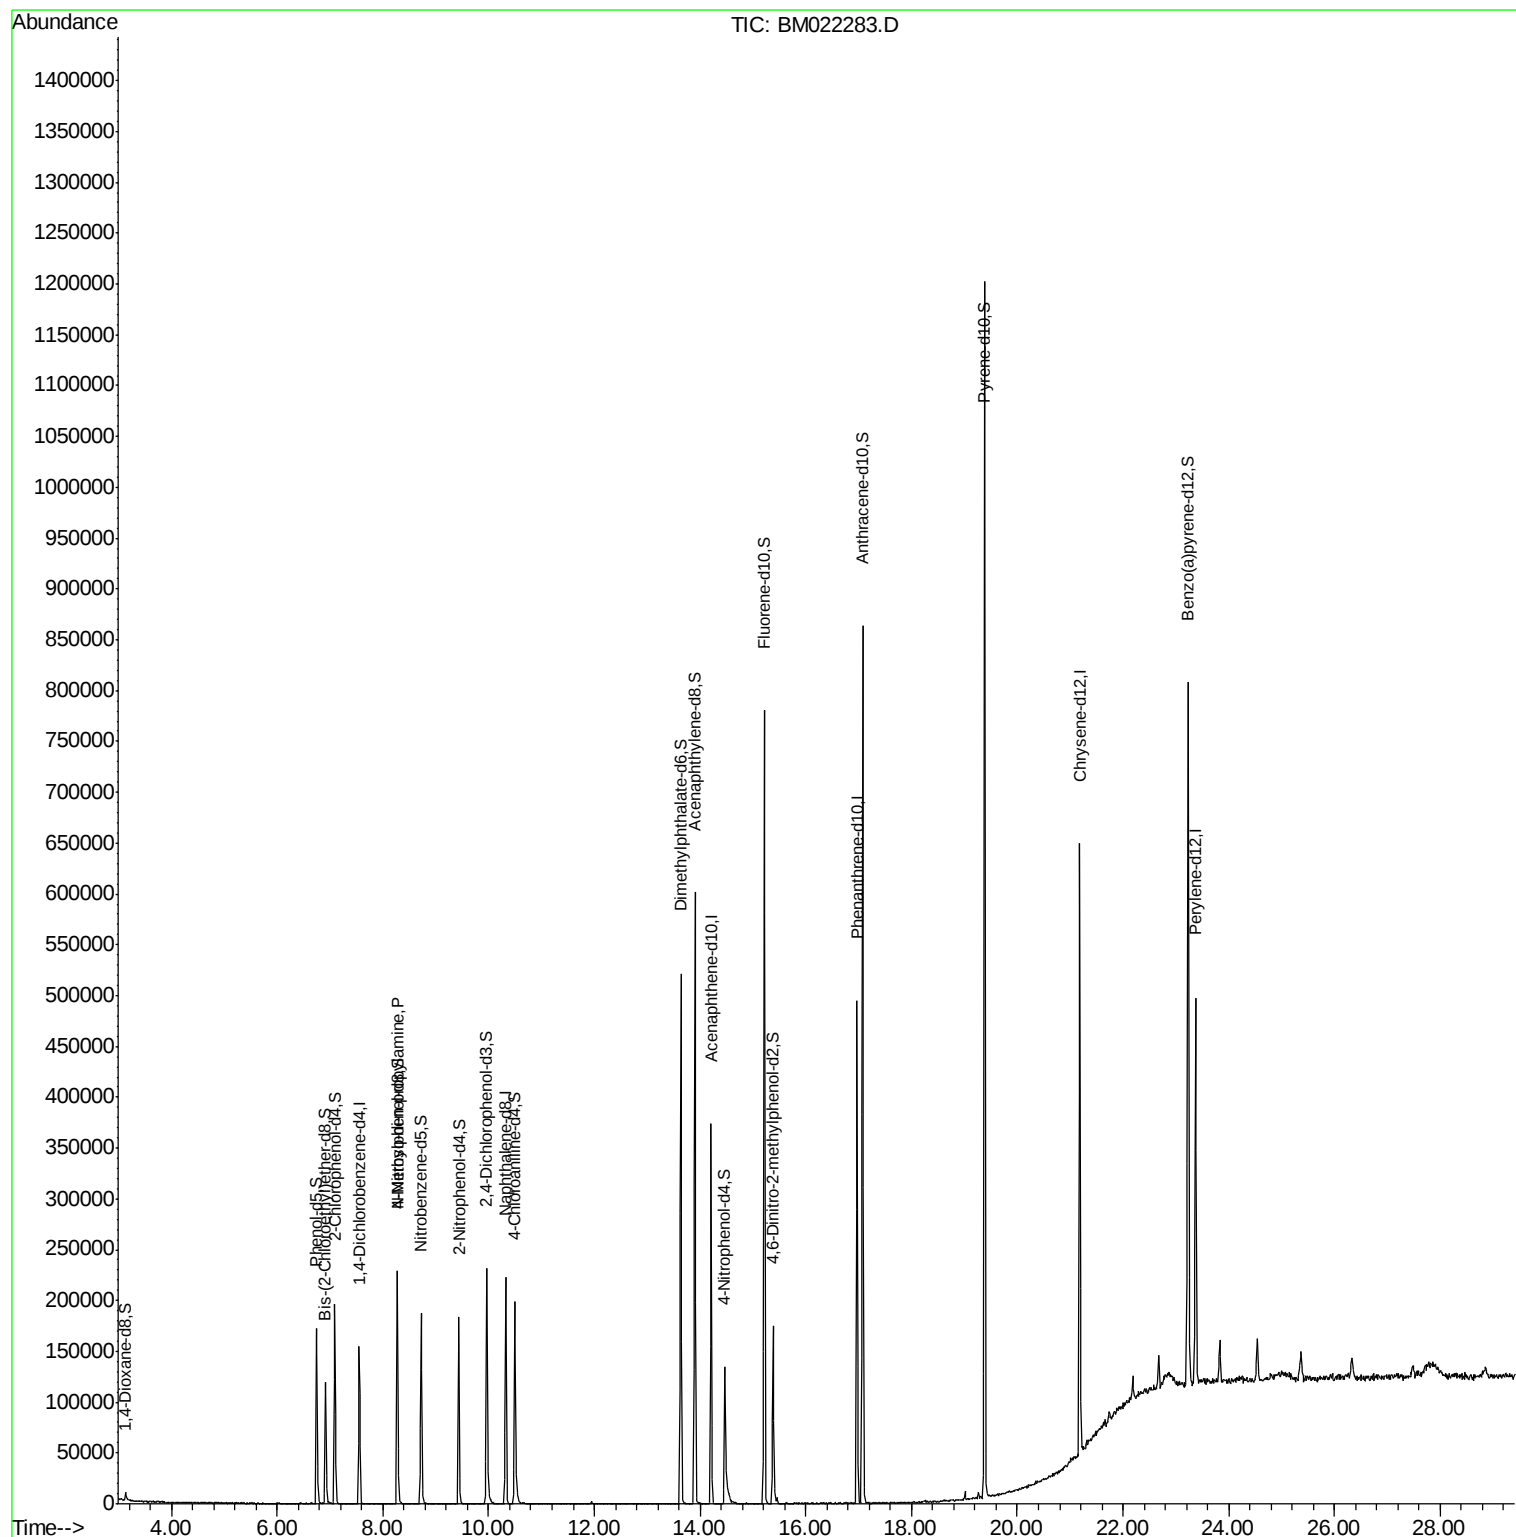

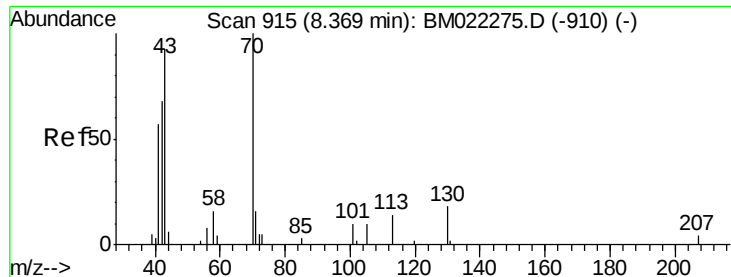

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.043 ng/ul
 RT: 8.27 min Scan# 898
 Delta R.T. -0.10 min
 Lab File: BM022283.D
 Acq: 24 Aug 2019 07:51

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Tgt Ion: 70 Resp: 2462
 Ion Ratio Lower Upper
 70 100
 42 377.3 55.1 82.7#
 101 0.0 8.0 12.0#
 130 0.0 15.7 23.5#

