

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
 Data File : BM022287.D
 Acq On : 24 Aug 2019 10:55
 Operator : HP/JU
 Sample : K4242-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ3

Quant Time: Aug 25 01:23:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 25 01:20:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	33351	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	149616	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	104182	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	242006	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	276549	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	250611	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	2155	2.89	ng/uL	0.00
5) Phenol-d5	6.75	99	42844	14.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	27674	16.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	38223	16.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	38102	15.27	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	19065	17.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	22076	17.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	41600	15.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	48377	15.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	152191	16.59	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	163931	16.59	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	13452	9.90	ng/ul	0.02
57) Fluorene-d10	15.22	176	127229	16.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	15671	8.39	ng/ul	0.00
70) Anthracene-d10	17.07	188	212723	16.60	ng/ul	0.00
78) Pyrene-d10	19.38	212	276639	19.25	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	230751	16.76	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.69	163	33195	3.556 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022287.D
Acq On : 24 Aug 2019 10:55
Operator : HP/JU
Sample : K4242-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ3

Quant Time: Aug 25 01:23:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 25 01:20:09 2019
Response via : Initial Calibration

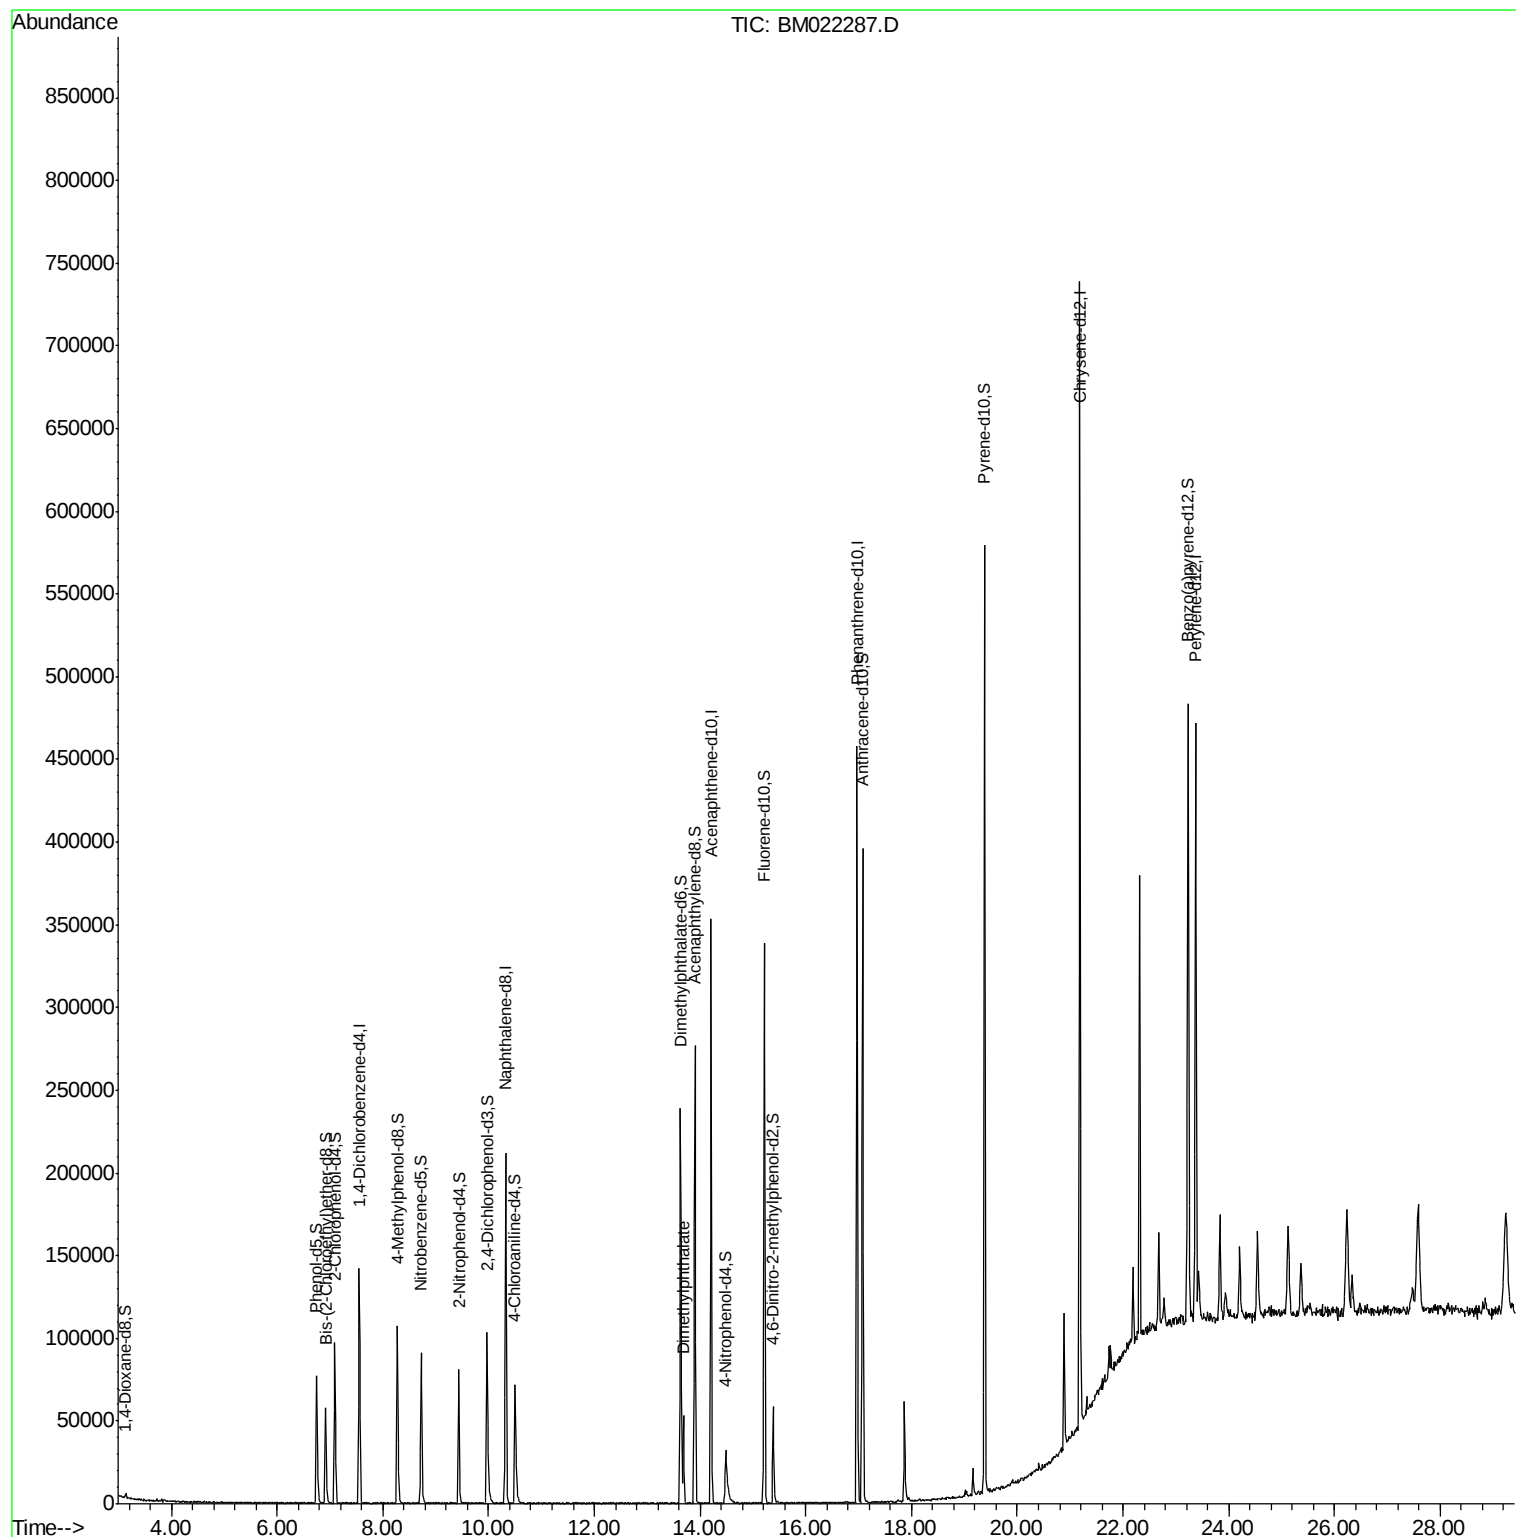

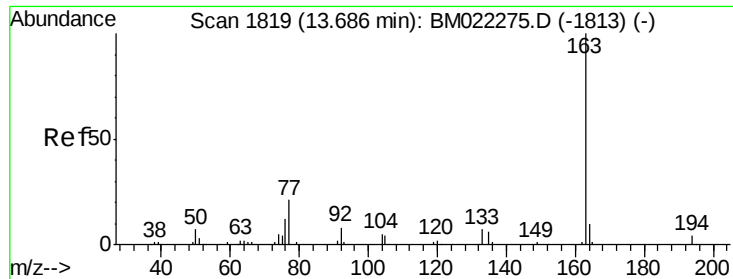

#44

Dimethylphthalate

Concen: 3.556 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM022287.D


Acq: 24 Aug 2019 10:55

Instrument :

BNA_M

ClientSampleId :

C0AJ3

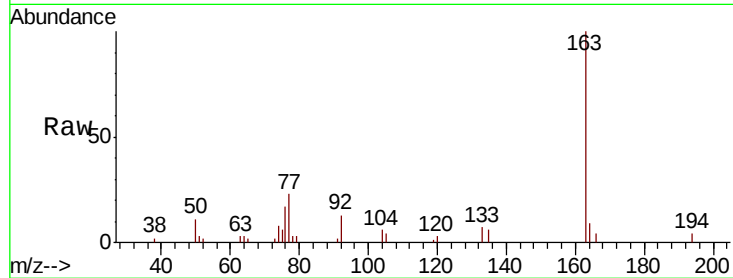

Tgt Ion:	163	Resp:	33195
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.6
164	9.1	7.8	11.8

