

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
 Data File : BM022305.D
 Acq On : 24 Aug 2019 21:57
 Operator : HP/JU
 Sample : PB122365BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Quant Time: Aug 25 02:24:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 25 02:20:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	25431	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	118576	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	83775	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	197096	20.00	ng/ul	0.00
77) Chrysene-d12	21.18	240	232901	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	218701	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	3155	5.55	ng/uL	0.00
5) Phenol-d5	6.75	99	64924	29.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	39754	31.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	57130	32.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	56744	29.83	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	27840	31.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	32982	32.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	63046	30.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	80408	31.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	220919	29.94	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	243541	30.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.48	143	23801	21.78	ng/ul	0.01
57) Fluorene-d10	15.22	176	192688	31.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	26048	17.13	ng/ul	0.00
70) Anthracene-d10	17.07	188	326982	31.33	ng/ul	0.00
78) Pyrene-d10	19.38	212	436462	36.06	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	378265	31.48	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.27	70	1794	1.078	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022305.D
Acq On : 24 Aug 2019 21:57
Operator : HP/JU
Sample : PB122365BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Time: Aug 25 02:24:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 25 02:20:02 2019
Response via : Initial Calibration

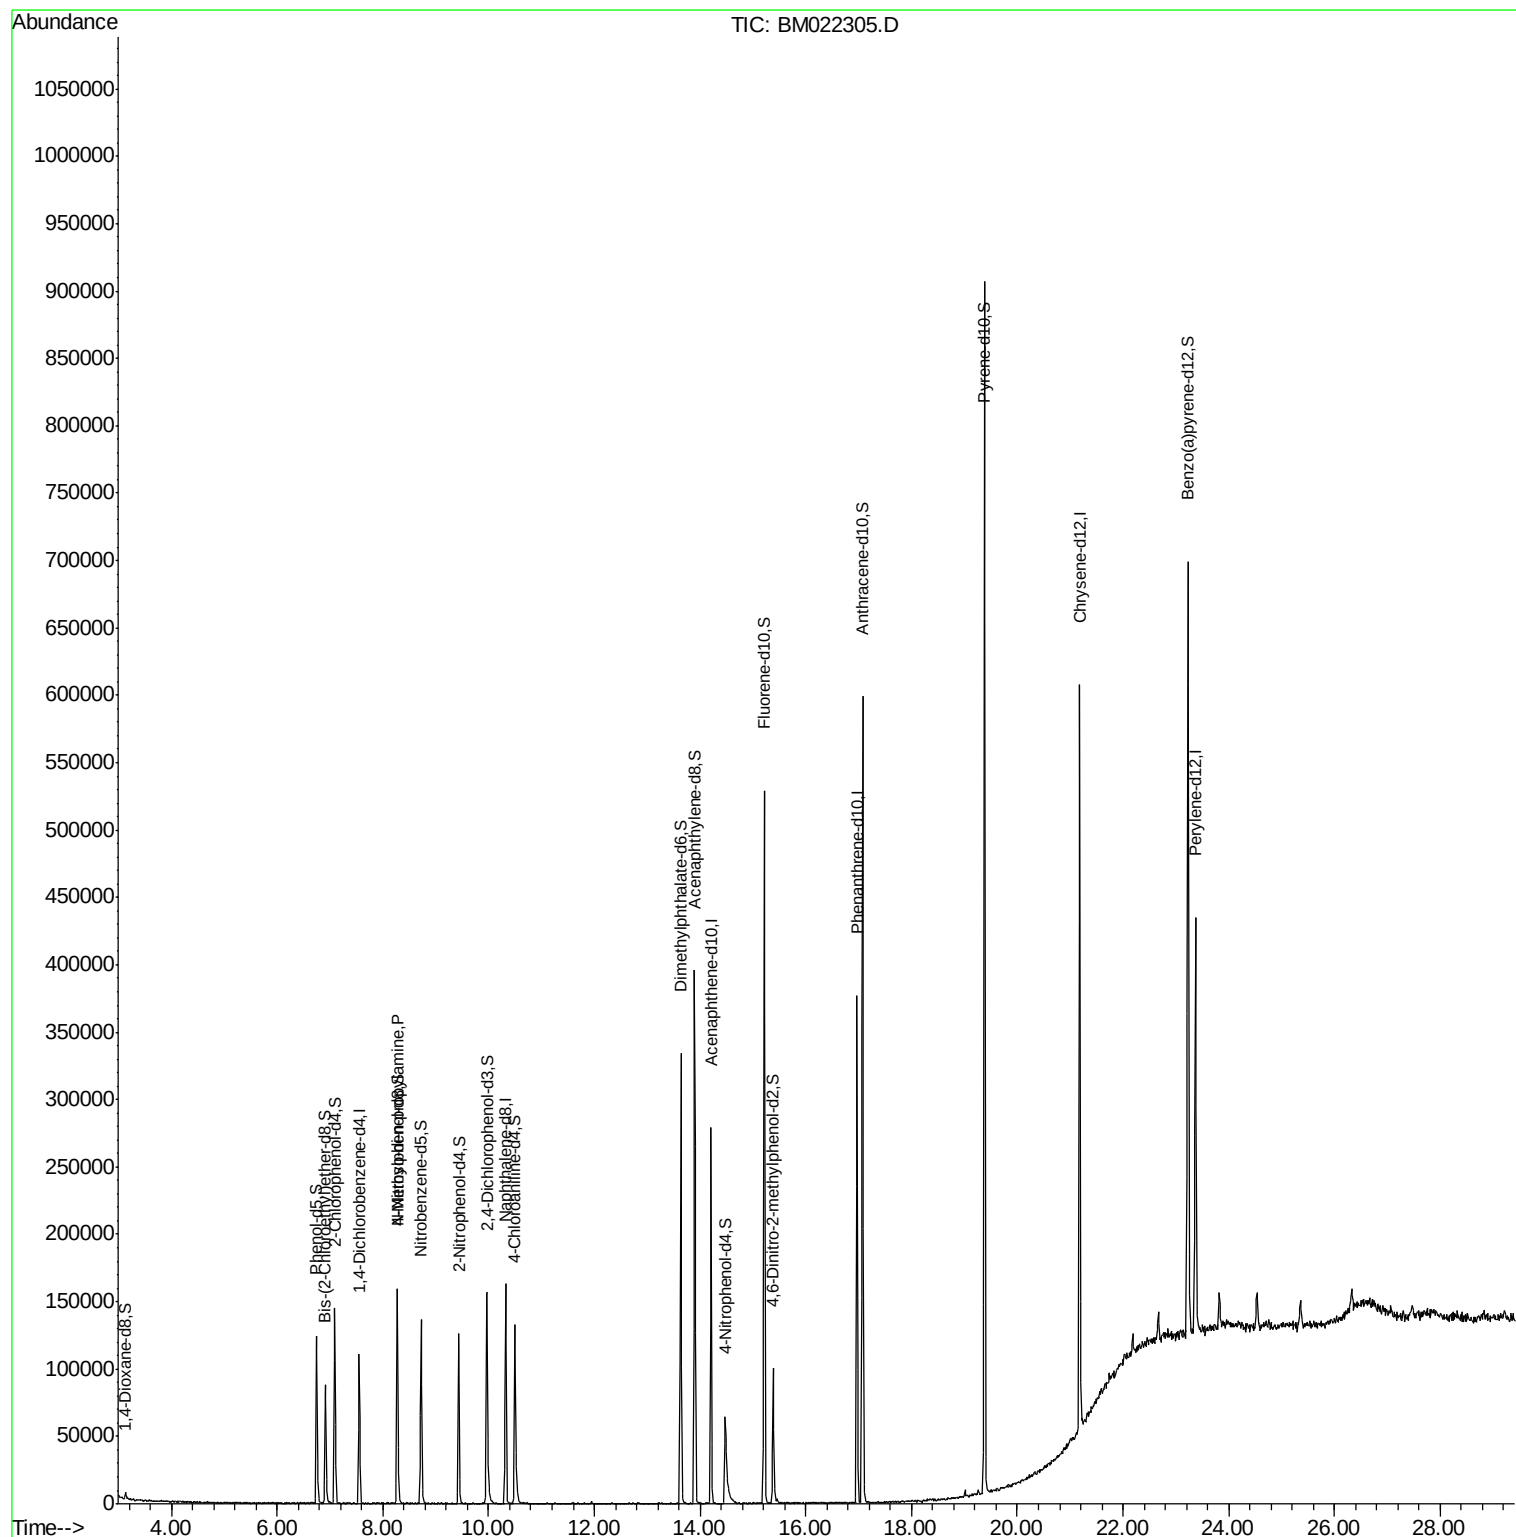

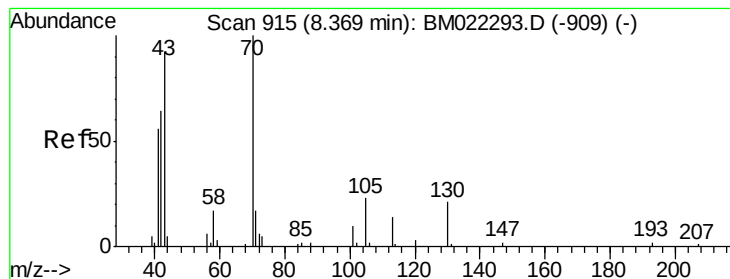

#15

N-Nitroso-di-n-propylamine

Concen: 1.078 ng/ul

RT: 8.27 min Scan# 898

Delta R.T. -0.10 min

Lab File: BM022305.D


Acq: 24 Aug 2019 21:57

Instrument :

BNA_M

ClientSampleId :

SBLK65

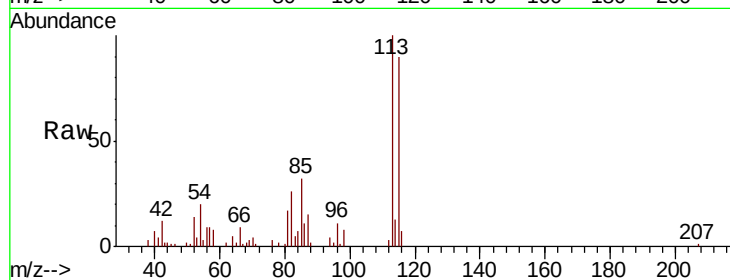

Tgt Ion: 70 Resp: 1794


Ion Ratio Lower Upper

70 100

42 331.6 55.1 82.7#

101 0.0 8.0 12.0#

130 0.0 15.7 23.5#

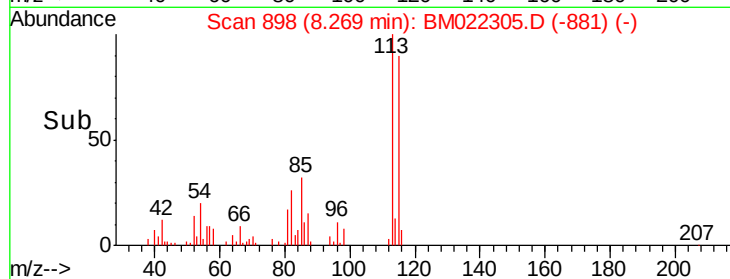

Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

