

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\

Data File : BM022249.D

Acq On : 23 Aug 2019 10:51

Operator : HP/JU

Sample : K4183-12

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 27 02:04:04 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Aug 22 19:41:45 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


C0AF0

Manual Integrations

APPROVED

mohammad

8/26/2019 8:29:21 AM

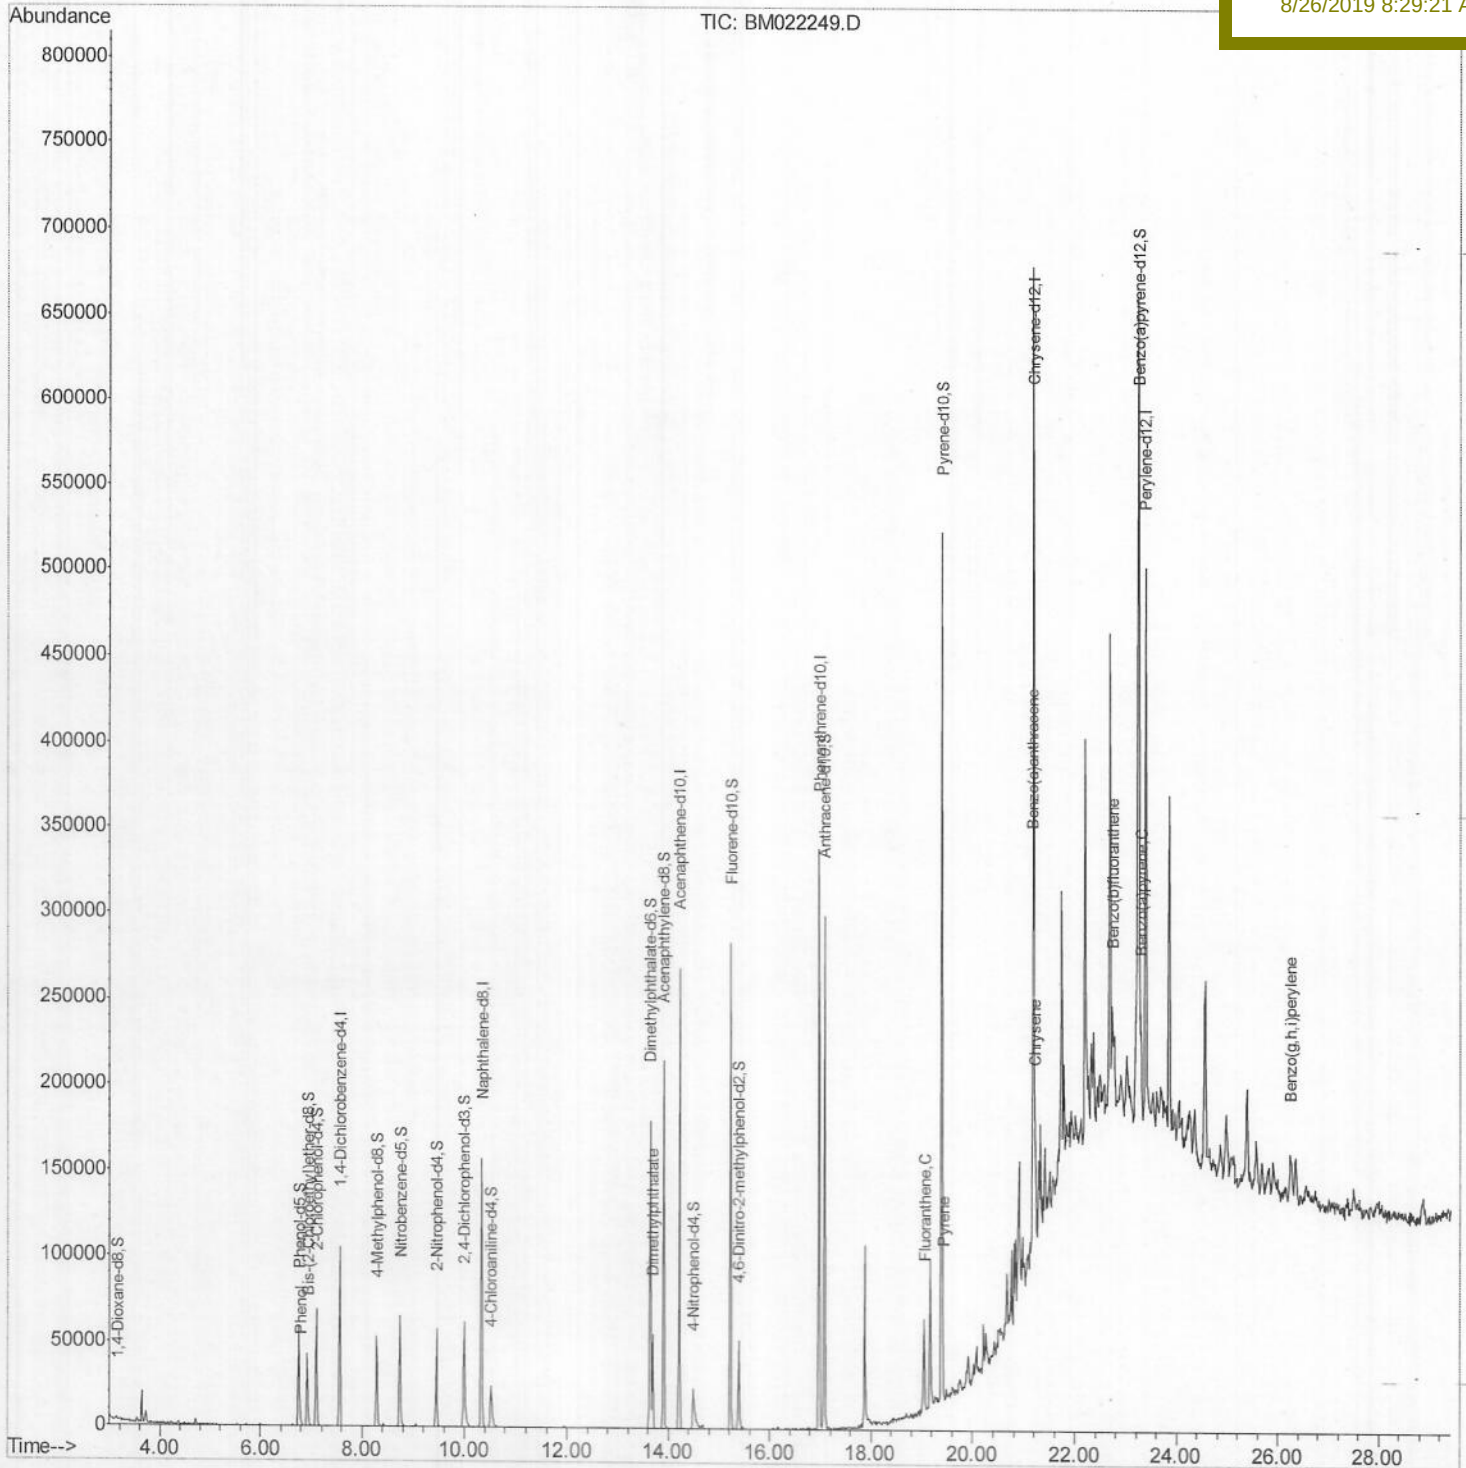

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022249.D
 Acq On : 23 Aug 2019 10:51
 Operator : HP/JU
 Sample : K4183-12
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual Integrations
 APPROVED

mohammad
 8/26/2019 8:29:21 AM

Quant Time: Aug 23 12:27:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 22 19:41:45 2019
 Response via : Initial Calibration

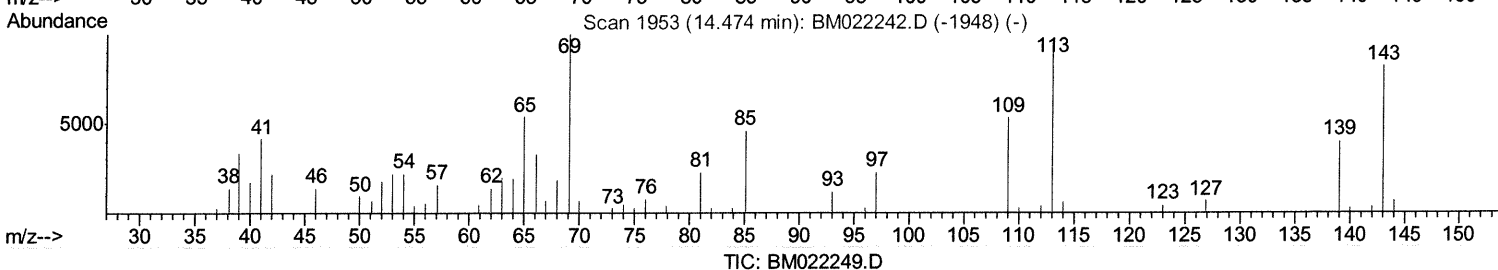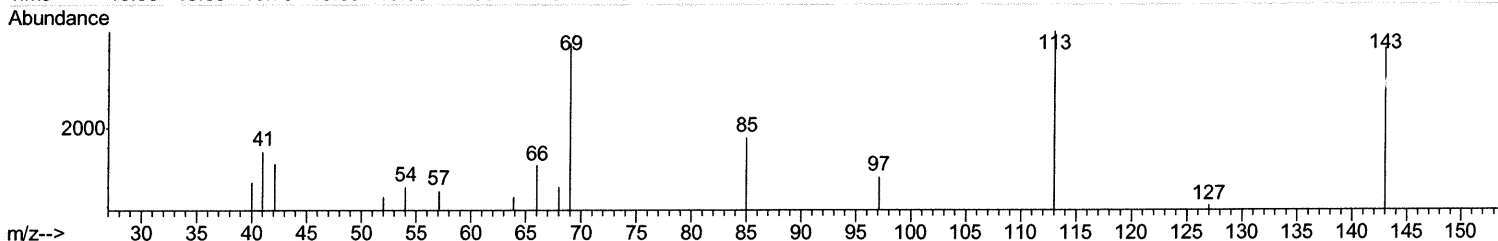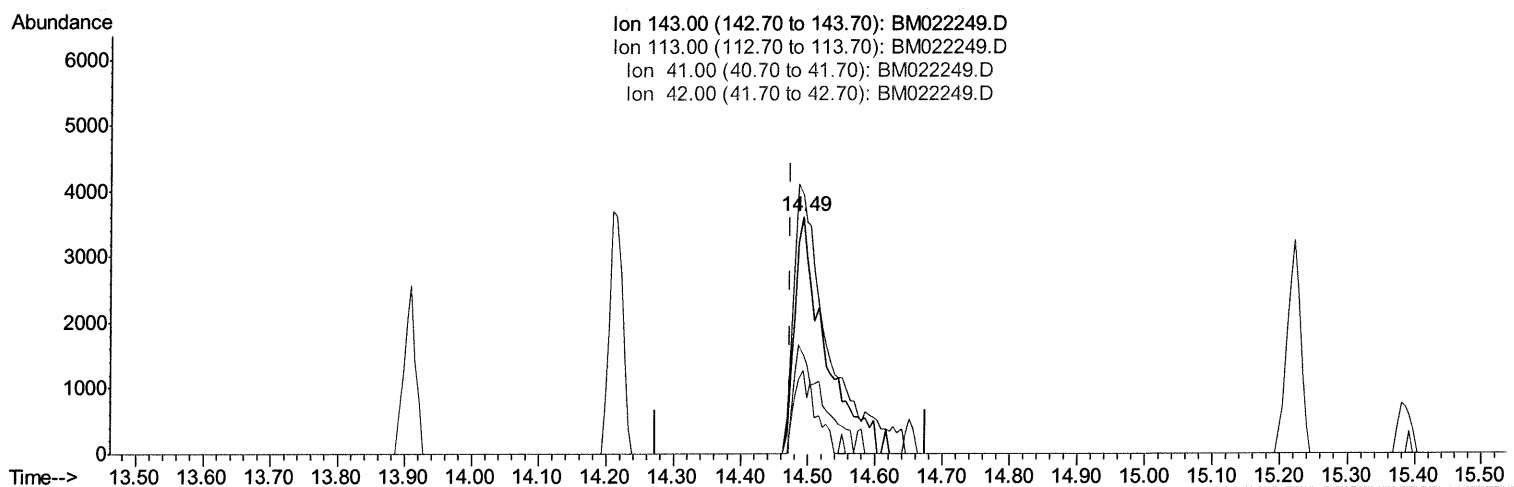

(51) 4-Nitrophenol-d4 (S)
 14.492min (+0.018) 9.00ng/ul
 response 9096

Ion	Exp%	Act%
143.00	100	100
113.00	116.00	109.98
41.00	50.80	42.18
42.00	27.00	35.11#

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022249.D
 Acq On : 23 Aug 2019 10:51
 Operator : HP/JU
 Sample : K4183-12
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual Integrations
 APPROVED

mohammad
 8/26/2019 8:29:21 AM

Quant Time: Aug 23 12:27:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 22 19:41:45 2019
 Response via : Initial Calibration

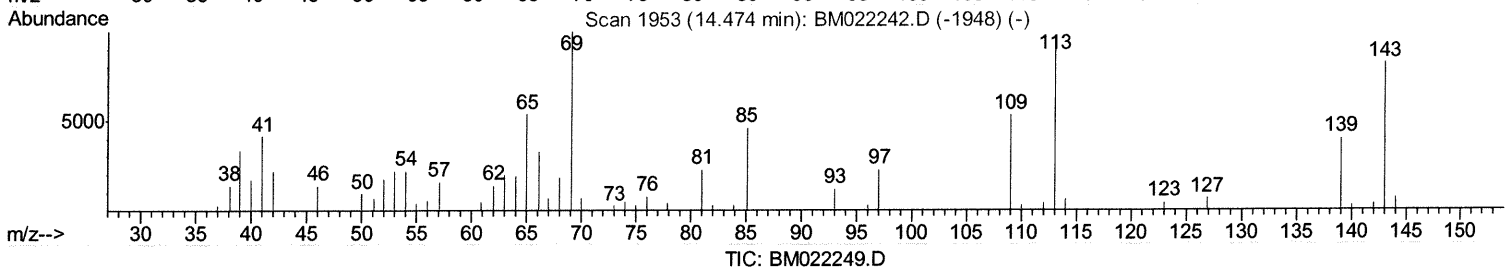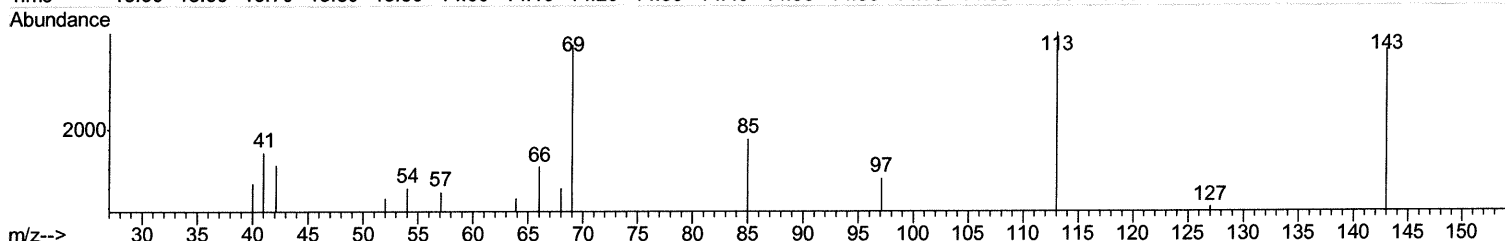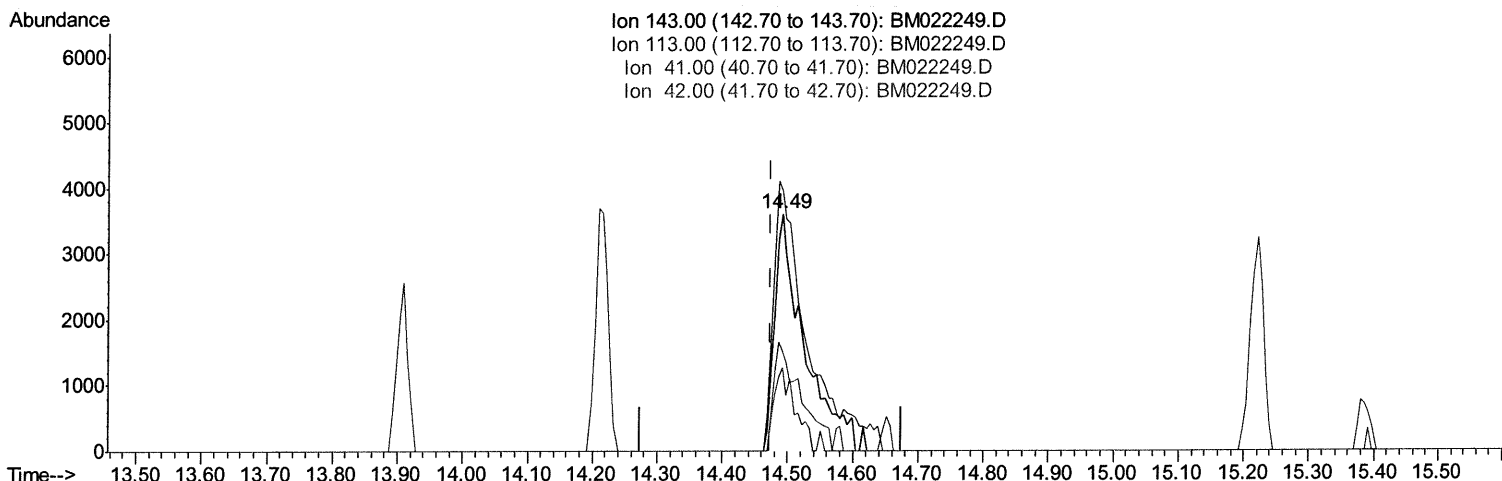

(51) 4-Nitrophenol-d4 (S)

14.492min (+0.018) 11.27ng/ul m

JU
 08/26/19

response 11398

Ion	Exp%	Act%
143.00	100	100
113.00	116.00	109.98
41.00	50.80	42.18
42.00	27.00	35.11#

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022249.D
 Acq On : 23 Aug 2019 10:51
 Operator : HP/JU
 Sample : K4183-12
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 27 02:04:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 22 19:41:45 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Manual Integrations
 APPROVED

mohammad
 8/26/2019 8:29:21 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	25576	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	114345	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	77506	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	182239	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	221941	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	204268	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	1041	1.82	ng/uL	0.00
5) Phenol-d5	6.75	99	32772	14.85	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.92	67	20124	15.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	28652	16.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	20115	10.51	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	13969	16.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	15009	15.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	30570	15.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	21938	8.93	ng/ul	0.02
43) Dimethylphthalate-d6	13.64	166	118067	17.30	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	123312	16.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	11398m	11.27	ng/ul	0.02
57) Fluorene-d10	15.22	176	101263	17.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	15546	11.06	ng/ul	0.00
70) Anthracene-d10	17.08	188	168945	17.51	ng/ul	0.00
78) Pyrene-d10	19.39	212	239709	20.78	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	217935	19.42	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.78	94	3446	1.458 ng/ul	92
44) Dimethylphthalate	13.69	163	34406	4.954 ng/ul	99
76) Fluoranthene	19.05	202	29283	1.782 ng/ul	98
79) Pyrene	19.42	202	29484	2.052 ng/ul	98
82) Benzo(a)anthracene	21.17	228	34742	2.080 ng/ul#	89
84) Chrysene	21.22	228	29944	1.917 ng/ul#	86
87) Benzo(b)fluoranthene	22.73	252	39274	2.764 ng/ul#	89
90) Benzo(a)pyrene	23.29	252	30823	2.276 ng/ul#	92
93) Benzo(a,h,i)perylene	26.25	276	17779	1.482 ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed