

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022258.D
 Acq On : 23 Aug 2019 16:22
 Operator : HP/JU
 Sample : K4337-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC8

Quant Time: Aug 23 17:06:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 23 13:10:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	24764	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	112321	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	78901	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	185074	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	223046	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	220281	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	593	1.07	ng/uL	0.00
5) Phenol-d5	6.76	99	17609	8.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	47812	38.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	55812	32.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	36951	19.95	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	35138	41.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	42244	43.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	75975	38.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	9135	3.79	ng/ul	0.03
43) Dimethylphthalate-d6	13.64	166	299756	43.14	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	311250	41.59	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	5770	5.61	ng/ul	0.04
57) Fluorene-d10	15.22	176	248441	43.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	48224	33.77	ng/ul	0.00
70) Anthracene-d10	17.08	188	431930	44.07	ng/ul	0.00
78) Pyrene-d10	19.39	212	585742	50.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	570158	47.11	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.69	163	30562	4.323	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022258.D
Acq On : 23 Aug 2019 16:22
Operator : HP/JU
Sample : K4337-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC8

Quant Time: Aug 23 17:06:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 23 13:10:05 2019
Response via : Initial Calibration

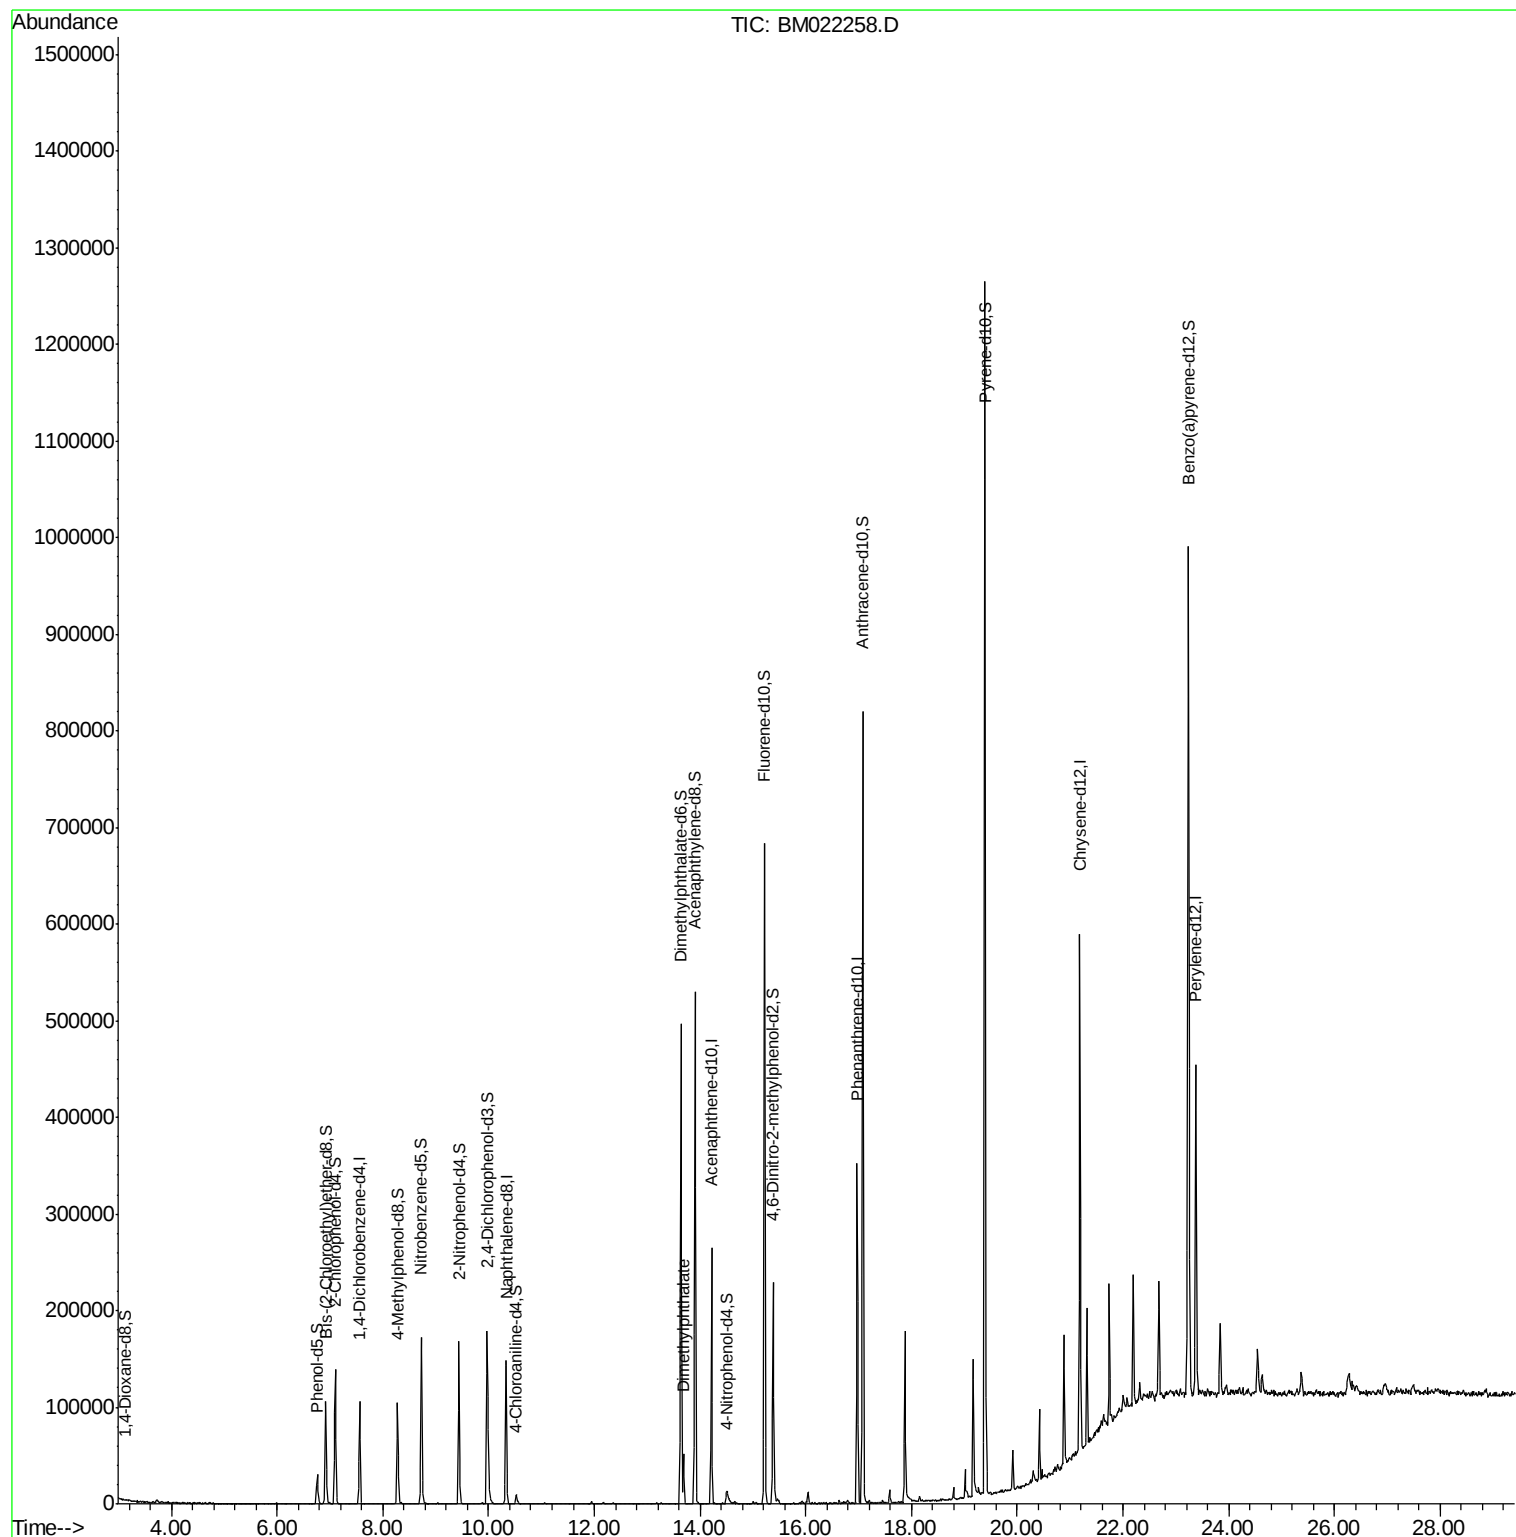

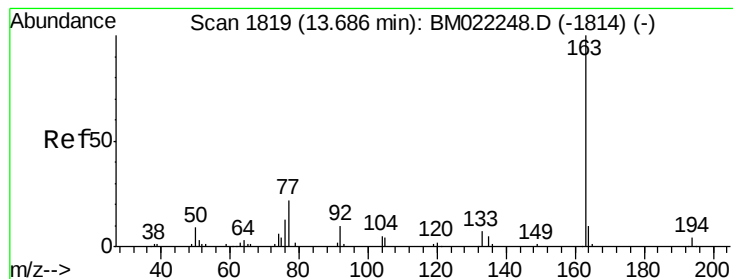

#44

Dimethylphthalate

Concen: 4.323 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM022258.D

Acq: 23 Aug 2019 16:22

Instrument :

BNA_M

ClientSampleId :

C0AC8


Tot Ion:163 Resp: 30562

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 9.5 7.8 11.8

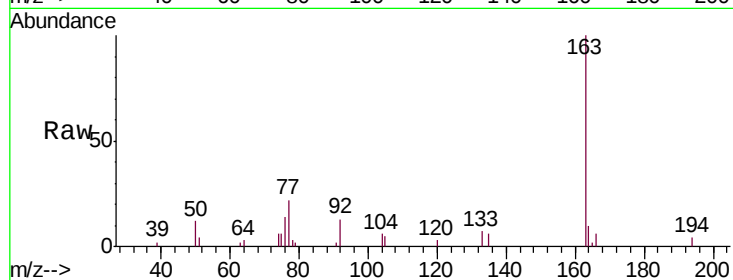

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

