

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022265.D
 Acq On : 23 Aug 2019 20:39
 Operator : HP/JU
 Sample : K4337-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA2

Quant Time: Aug 24 01:12:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 24 01:09:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	27550	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	124870	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	89636	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	211792	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	275685	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	289932	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.76	99	6913	2.91	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.92	67	20494	14.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	23871	12.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	16082	7.80	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	14507	15.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	16844	15.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	31840	14.43	ng/ul	0.01
29) 4-Chloroaniline-d4	10.54	131	2563	0.96	ng/ul	0.04
43) Dimethylphthalate-d6	13.64	166	136121	17.24	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	139761	16.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	1581	1.35	ng/ul	0.05
57) Fluorene-d10	15.22	176	112727	17.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	19146	11.72	ng/ul	0.00
70) Anthracene-d10	17.07	188	198074	17.66	ng/ul	0.00
78) Pyrene-d10	19.38	212	271226	18.93	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	286546	17.99	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	25463	3.170	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022265.D
Acq On : 23 Aug 2019 20:39
Operator : HP/JU
Sample : K4337-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA2

Quant Time: Aug 24 01:12:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 24 01:09:04 2019
Response via : Initial Calibration

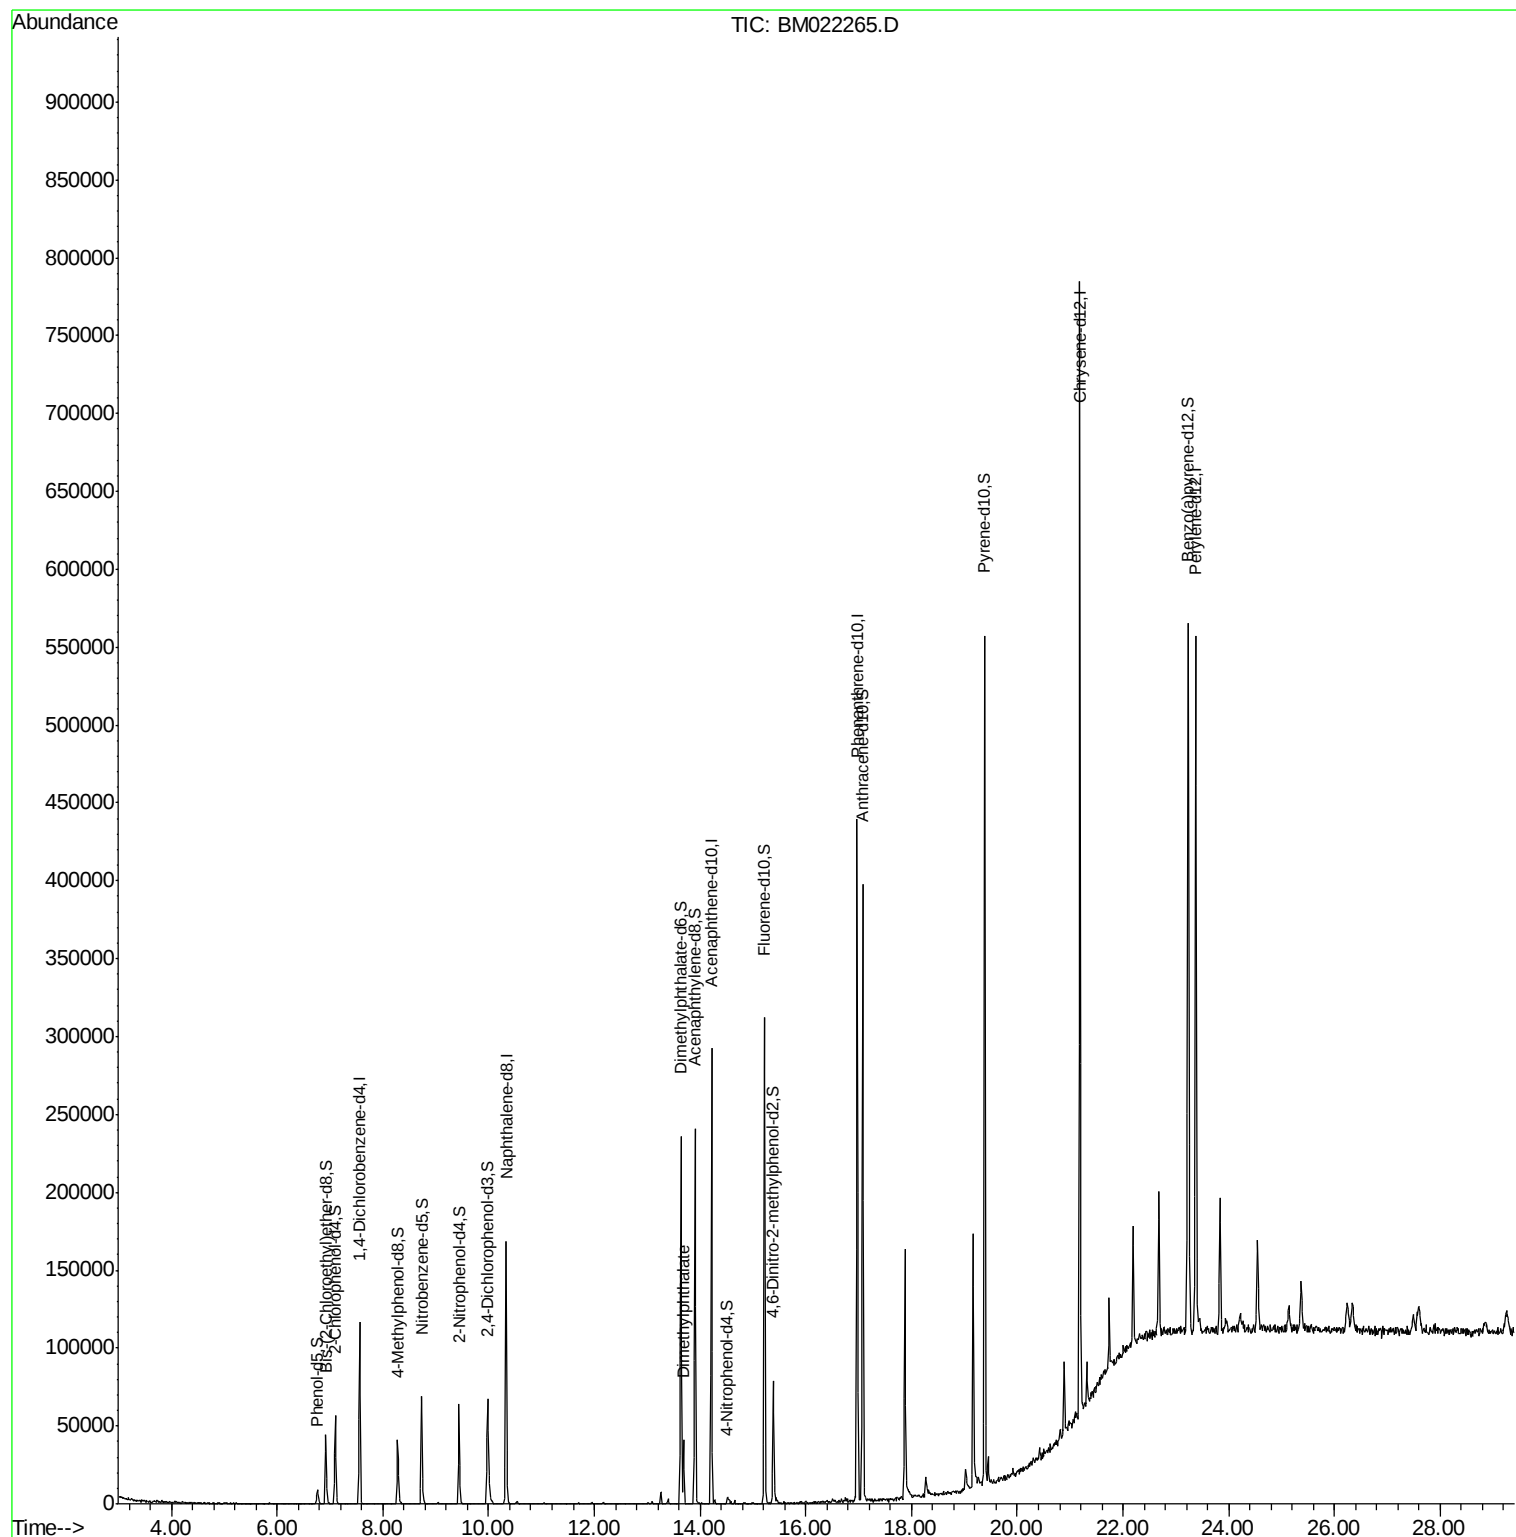

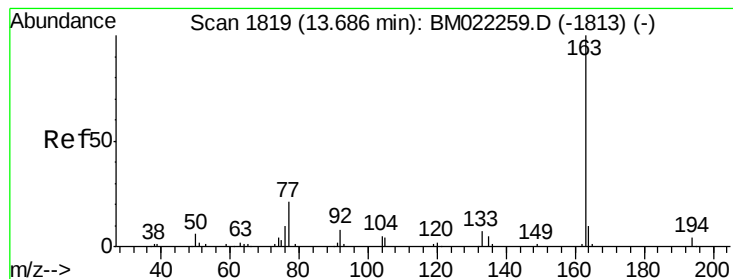

#44

Dimethylphthalate

Concen: 3.170 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM022265.D

Acq: 23 Aug 2019 20:39

Instrument :

BNA_M

ClientSampleId :

C0AA2

Tot Ion:163 Resp: 25463

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 9.8 7.8 11.8

