

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022269.D
 Acq On : 23 Aug 2019 23:08
 Operator : HP/JU
 Sample : K4337-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB8

Quant Time: Aug 24 01:13:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 24 01:09:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	27911	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	125950	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	89743	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	211412	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	264913	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	270780	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	638	1.02	ng/uL	0.00
5) Phenol-d5	6.76	99	17418	7.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	43681	31.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	49823	25.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	34544	16.55	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	30818	32.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.44	143	35951	32.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	66273	29.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	6169	2.28	ng/ul	0.03
43) Dimethylphthalate-d6	13.64	166	264801	33.51	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	277431	32.59	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	4659	3.98	ng/ul	0.03
57) Fluorene-d10	15.22	176	221595	33.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	39566	24.25	ng/ul	0.00
70) Anthracene-d10	17.07	188	389927	34.83	ng/ul	0.00
78) Pyrene-d10	19.39	212	538930	39.14	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	557521	37.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	50044	6.223	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022269.D
Acq On : 23 Aug 2019 23:08
Operator : HP/JU
Sample : K4337-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB8

Quant Time: Aug 24 01:13:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 24 01:09:04 2019
Response via : Initial Calibration

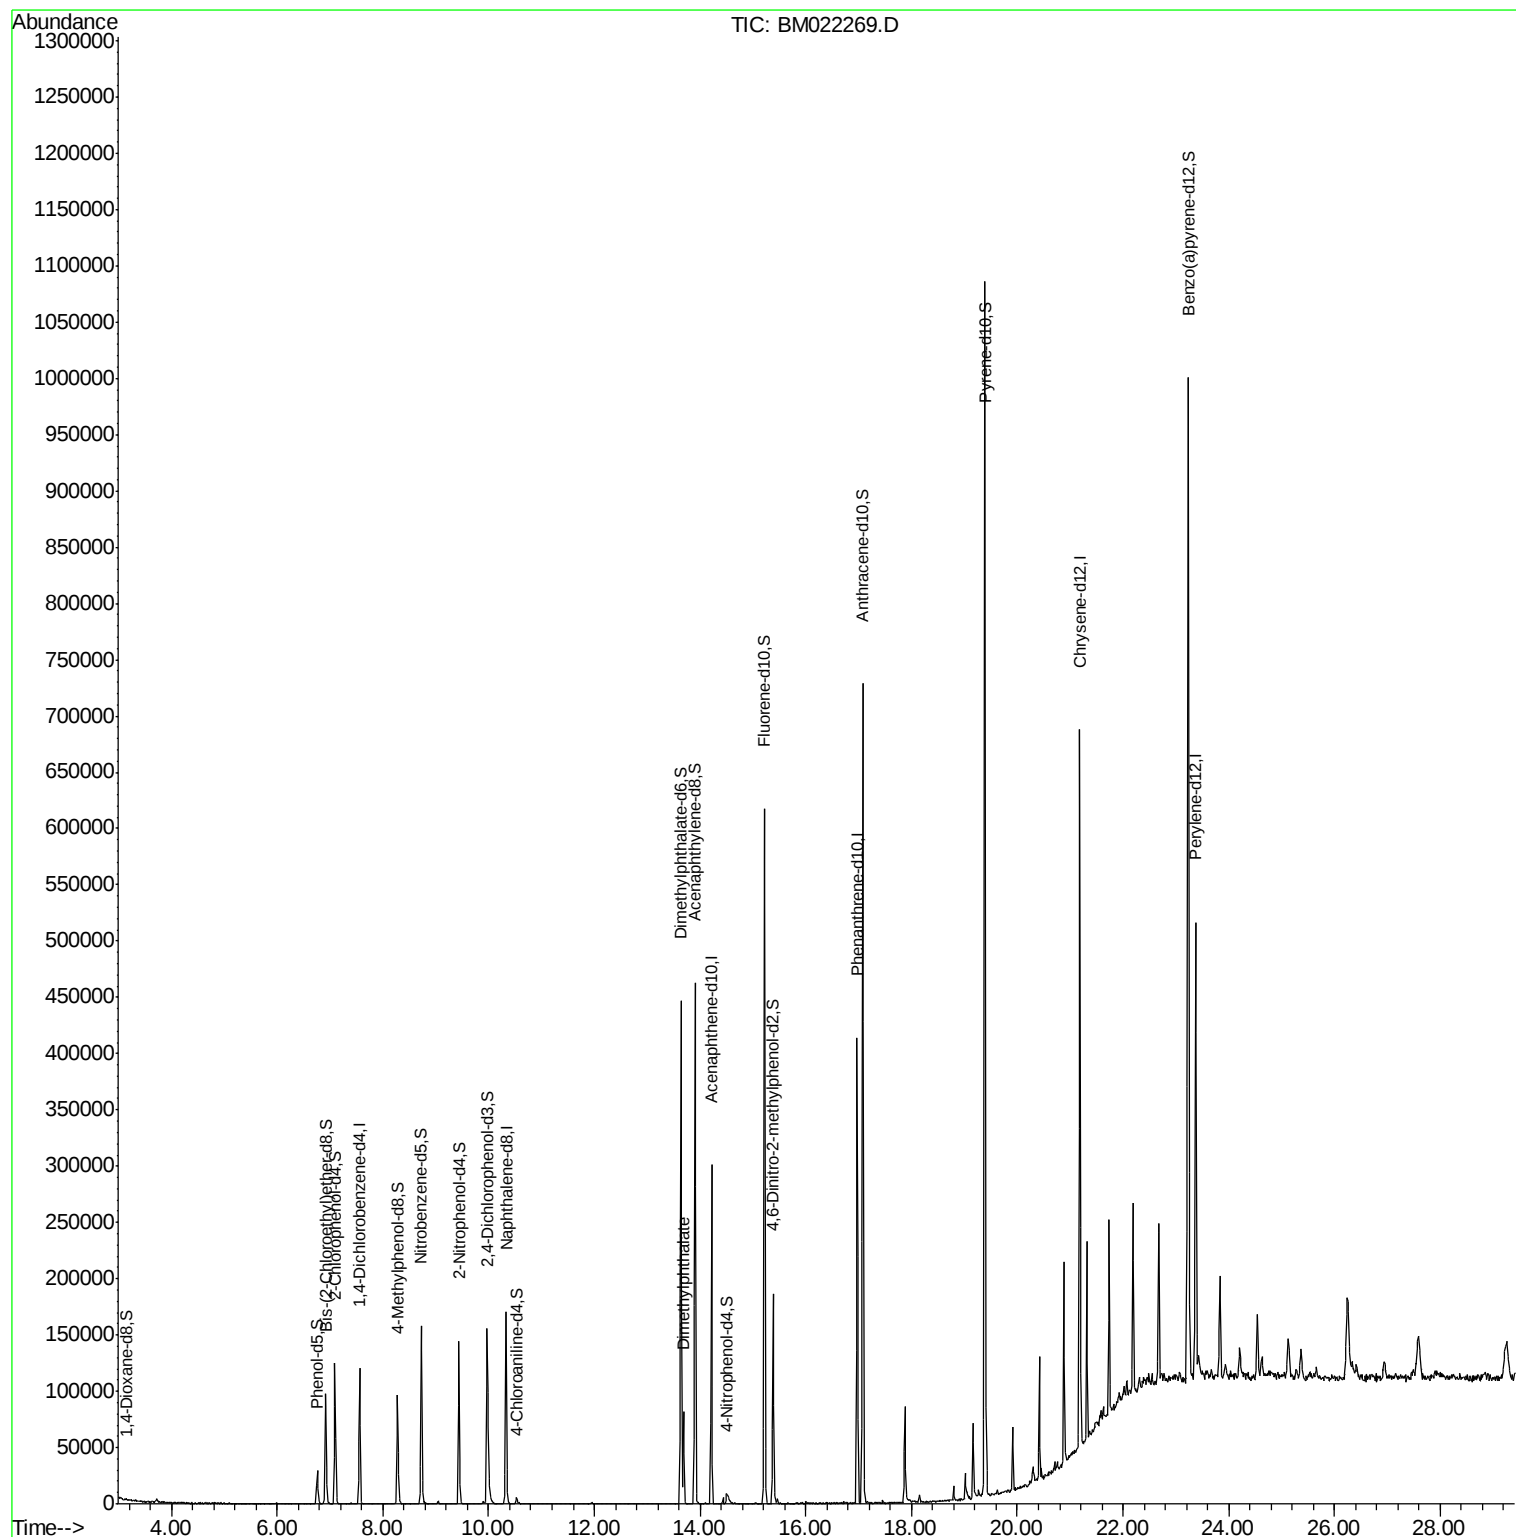

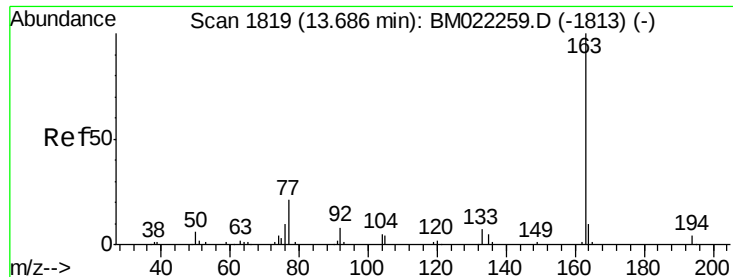

#44

Dimethylphthalate

Concen: 6.223 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. 0.00 min

Lab File: BM022269.D

Acq: 23 Aug 2019 23:08

Instrument :

BNA_M

ClientSampleId :

C0AB8


Tot Ion:163 Resp: 50044

Ion Ratio Lower Upper

163 100

194 4.6 3.0 4.6

164 10.2 7.8 11.8

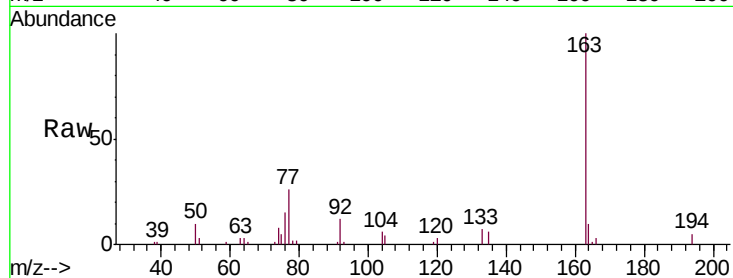

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

