

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022294.D
 Acq On : 24 Aug 2019 15:12
 Operator : HP/JU
 Sample : K4337-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA2

Quant Time: Aug 25 02:23:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 25 02:20:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	33295	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	149301	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	101182	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	230992	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	239110	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	204150	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	2302	3.09	ng/uL	0.00
5) Phenol-d5	6.75	99	29756	10.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	38708	23.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	48340	20.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	40942	16.44	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	29013	26.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	35425	27.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	67107	25.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	31234	9.74	ng/ul	0.01
43) Dimethylphthalate-d6	13.64	166	248043	27.84	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	276263	28.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	11741	8.89	ng/ul	0.03
57) Fluorene-d10	15.22	176	210872	28.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	30542	17.14	ng/ul	0.00
70) Anthracene-d10	17.07	188	358373	29.30	ng/ul	0.00
78) Pyrene-d10	19.38	212	453991	36.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	336519	30.00	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.69	163	31758	3.503	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022294.D
Acq On : 24 Aug 2019 15:12
Operator : HP/JU
Sample : K4337-11
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA2

Quant Time: Aug 25 02:23:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 25 02:20:02 2019
Response via : Initial Calibration

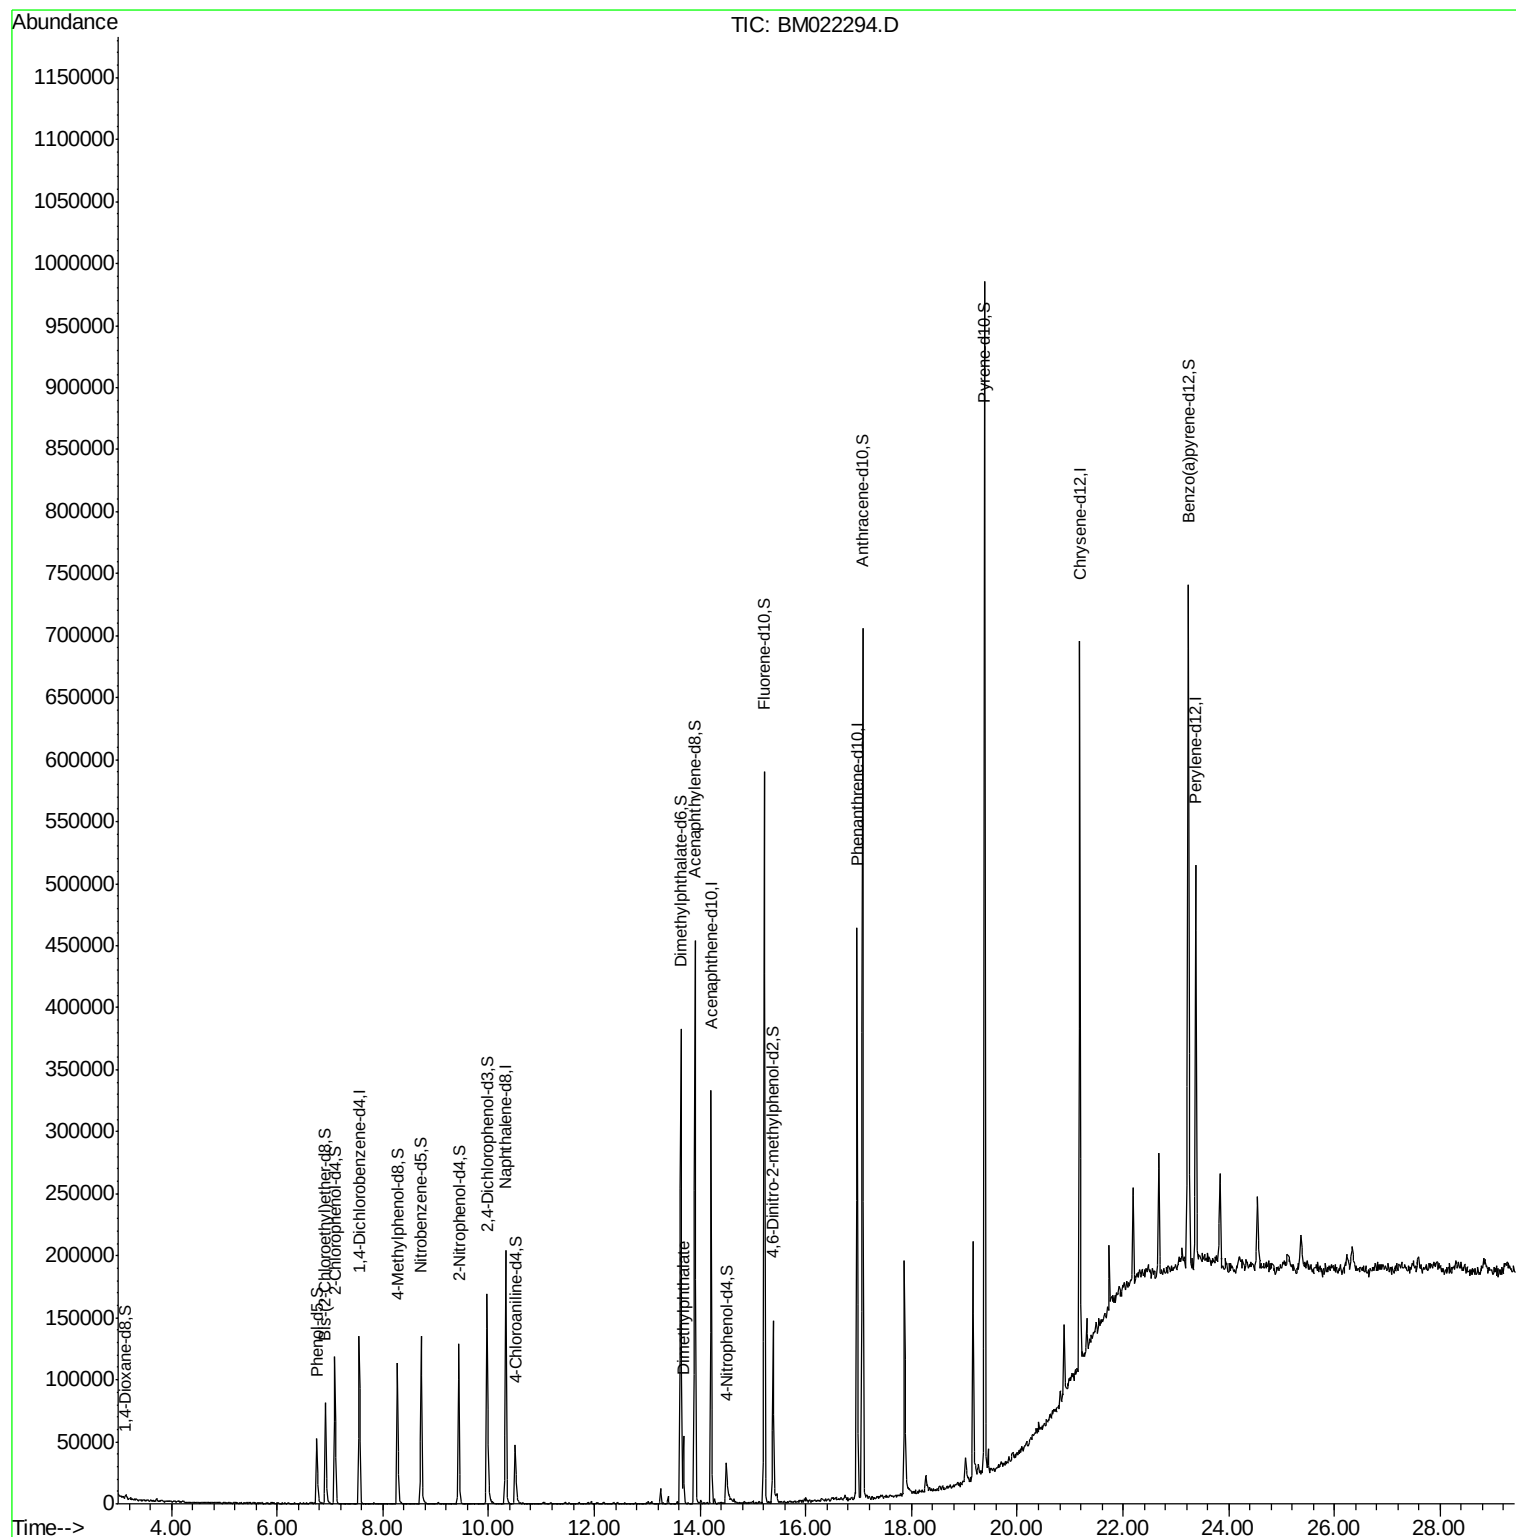

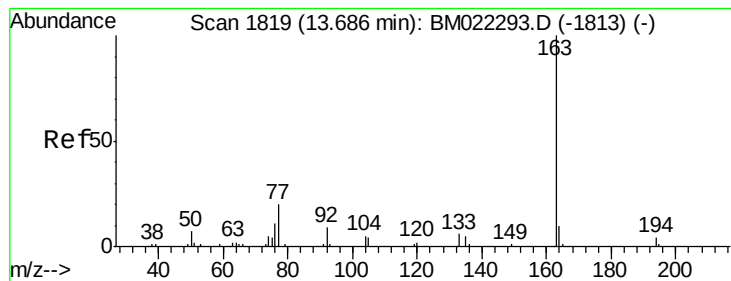

#44

Dimethylphthalate

Concen: 3.503 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.00 min

Lab File: BM022294.D

Acq: 24 Aug 2019 15:12

Instrument :

BNA_M

ClientSampleId :

C0AA2


Tot Ion:163 Resp: 31758

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6

164 10.1 7.8 11.8

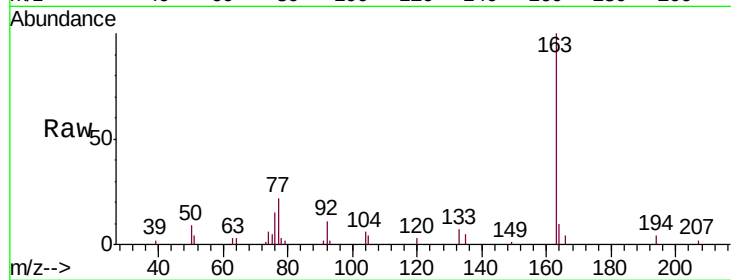

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

