

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022271.D
 Acq On : 24 Aug 2019 00:22
 Operator : HP/JU
 Sample : K4397-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	28	30	33	rBV2	705	709	0.13%	0.033%
2	3.228	38	41	42	rVV2	617	668	0.12%	0.031%
3	3.417	71	73	76	rBV3	1189	1614	0.29%	0.076%
4	3.458	78	80	83	rVB2	829	701	0.13%	0.033%
5	3.481	83	84	87	rBV	949	675	0.12%	0.032%
6	3.605	103	105	109	rVB2	664	824	0.15%	0.039%
7	3.699	120	121	125	rVB	840	694	0.13%	0.032%
8	3.775	133	134	137	rVB	804	610	0.11%	0.029%
9	3.840	142	145	147	rBV2	728	645	0.12%	0.030%
10	3.875	149	151	153	rBV2	962	1157	0.21%	0.054%
11	3.999	171	172	176	rVB	838	925	0.17%	0.043%
12	4.158	194	199	202	rBV2	649	1054	0.19%	0.049%
13	4.217	207	209	210	rBV2	612	558	0.10%	0.026%
14	4.258	213	216	219	rVB2	723	824	0.15%	0.039%
15	4.322	226	227	230	rBV	845	619	0.11%	0.029%
16	4.364	230	234	236	rVB	577	618	0.11%	0.029%
17	4.381	236	237	239	rBV	836	659	0.12%	0.031%
18	4.405	239	241	244	rVB	760	723	0.13%	0.034%
19	4.487	251	255	256	rVB2	489	602	0.11%	0.028%
20	4.581	269	271	273	rVB	1117	770	0.14%	0.036%
21	4.617	273	277	278	rBB	723	765	0.14%	0.036%
22	4.640	278	281	284	rBV	803	1010	0.18%	0.047%
23	4.670	284	286	289	rVV	763	1061	0.19%	0.050%
24	4.711	291	293	296	rBB2	704	805	0.15%	0.038%
25	4.793	306	307	310	rBB2	710	728	0.13%	0.034%
26	4.887	320	323	325	rVB2	456	577	0.10%	0.027%
27	4.952	332	334	336	rBV	675	606	0.11%	0.028%
28	4.999	338	342	345	rVB	739	895	0.16%	0.042%
29	5.046	348	350	352	rBB	704	605	0.11%	0.028%
30	7.558	772	777	791	rBV	71594	130386	23.70%	6.101%
31	10.334	1243	1249	1264	rBV	94059	190926	34.71%	8.933%
32	14.216	1903	1909	1925	rBB2	183900	304696	55.39%	14.256%
33	15.857	2187	2188	2191	rBB	646	558	0.10%	0.026%
34	16.239	2251	2253	2256	rBB	628	583	0.11%	0.027%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022271.D
 Acq On : 24 Aug 2019 00:22
 Operator : HP/JU
 Sample : K4397-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	16.716	2332	2334	2337	rBV	407	639	0.12%	0.030%
36	16.769	2341	2343	2344	rBV	924	657	0.12%	0.031%
37	16.810	2348	2350	2352	rBV	647	682	0.12%	0.032%
38	16.886	2362	2363	2368	rVB	706	724	0.13%	0.034%
39	16.980	2373	2379	2392	rBV	232870	384294	69.86%	17.981%
40	17.210	2413	2418	2422	rBV2	605	991	0.18%	0.046%
41	17.263	2422	2427	2429	rBV	680	658	0.12%	0.031%
42	17.363	2441	2444	2445	rBV	691	666	0.12%	0.031%
43	17.698	2500	2501	2507	rBV	612	898	0.16%	0.042%
44	17.886	2530	2533	2534	rBV2	1105	732	0.13%	0.034%
45	17.927	2538	2540	2542	rVV2	676	612	0.11%	0.029%
46	17.957	2544	2545	2548	rVV2	745	692	0.13%	0.032%
47	18.122	2571	2573	2576	rVB	646	708	0.13%	0.033%
48	18.157	2576	2579	2580	rBV	942	892	0.16%	0.042%
49	18.251	2594	2595	2597	rBV	1087	815	0.15%	0.038%
50	18.286	2597	2601	2603	rVV	1024	1218	0.22%	0.057%
51	18.304	2603	2604	2608	rVB	832	962	0.17%	0.045%
52	18.510	2637	2639	2642	rVB	748	744	0.14%	0.035%
53	18.539	2642	2644	2645	rBV	1277	659	0.12%	0.031%
54	18.586	2651	2652	2654	rVB	983	609	0.11%	0.028%
55	18.622	2654	2658	2660	rBV	1503	1723	0.31%	0.081%
56	18.680	2666	2668	2670	rBV	1149	1084	0.20%	0.051%
57	18.769	2681	2683	2685	rVV2	907	768	0.14%	0.036%
58	18.992	2717	2721	2723	rBV3	956	1373	0.25%	0.064%
59	19.051	2727	2731	2733	rBV3	1057	1439	0.26%	0.067%
60	19.110	2739	2741	2744	rVB3	1040	944	0.17%	0.044%
61	19.139	2744	2746	2749	rBV3	1009	823	0.15%	0.039%
62	19.222	2759	2760	2762	rVB2	1992	1078	0.20%	0.050%
63	19.245	2762	2764	2765	rBV2	880	620	0.11%	0.029%
64	19.274	2767	2769	2771	rVV2	1366	1302	0.24%	0.061%
65	19.298	2771	2773	2775	rVV2	1263	642	0.12%	0.030%
66	19.322	2775	2777	2781	rBV3	854	1351	0.25%	0.063%
67	19.357	2781	2783	2784	rVV	1466	911	0.17%	0.043%
68	19.386	2786	2788	2790	rVB2	1168	735	0.13%	0.034%
69	19.410	2790	2792	2793	rBV2	953	822	0.15%	0.038%
70	19.492	2804	2806	2809	rBV3	1782	2112	0.38%	0.099%
71	19.522	2809	2811	2812	rBV	1263	770	0.14%	0.036%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022271.D
Acq On : 24 Aug 2019 00:22
Operator : HP/JU
Sample : K4397-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Title : SVOA CALIBRATION

72	19.686	2838	2839	2842	rBV3	1138	992	0.18%	0.046%
73	19.745	2847	2849	2851	rBV3	1643	1127	0.20%	0.053%
74	21.186	3089	3094	3104	rBV	392602	550100	100.00%	25.739%
75	23.374	3460	3466	3482	rVB	255550	517845	94.14%	24.229%


Sum of corrected areas: 2137263

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022271.D
Acq On : 24 Aug 2019 00:22
Operator : HP/JU
Sample : K4397-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

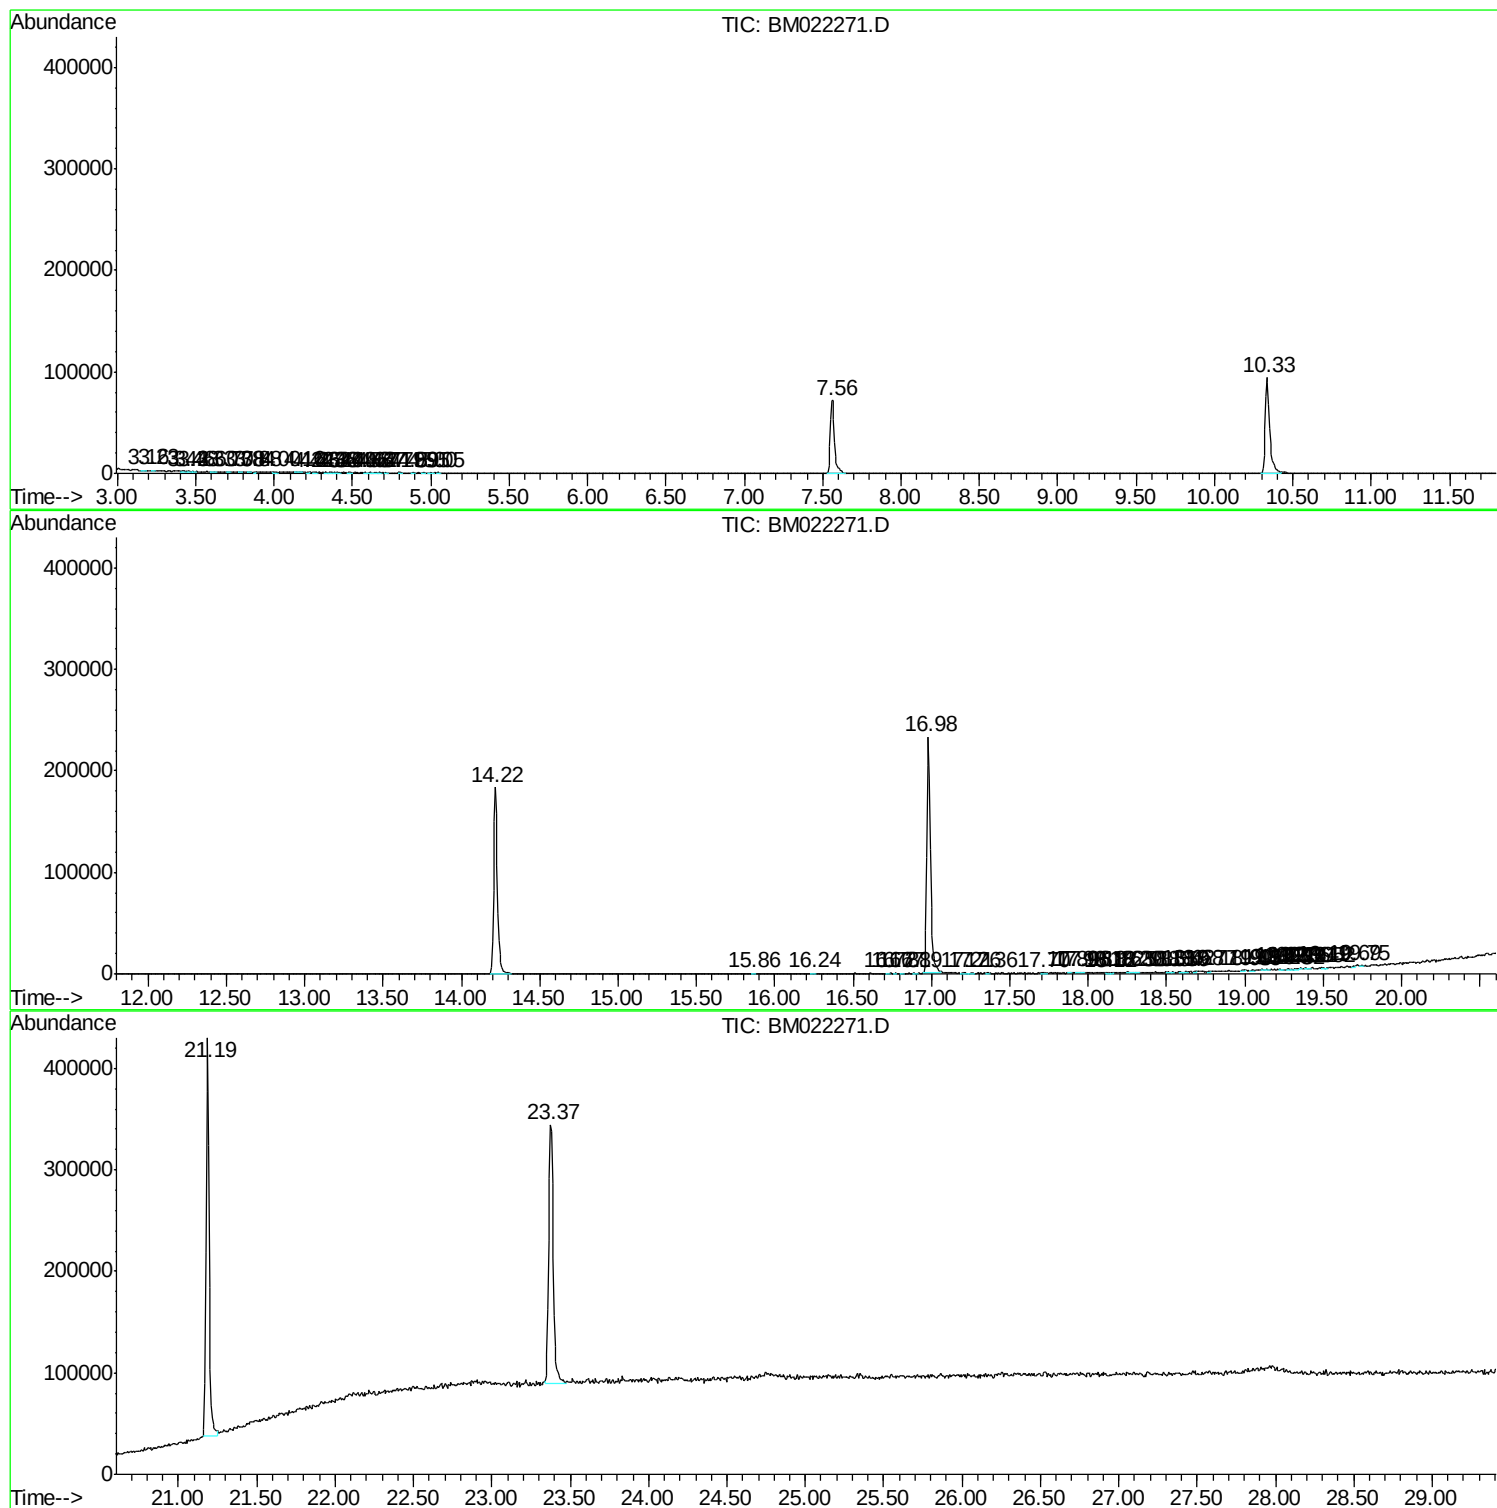

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022271.D
Acq On : 24 Aug 2019 00:22
Operator : HP/JU
Sample : K4397-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022271.D
Acq On : 24 Aug 2019 00:22
Operator : HP/JU
Sample : K4397-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
