

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022283.D
 Acq On : 24 Aug 2019 07:51
 Operator : HP/JU
 Sample : PB122365BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	30	rVB	7744	10566	0.68%	0.080%
2	6.746	634	639	651	rBV	172266	289329	18.64%	2.201%
3	6.910	662	667	680	rBV	119620	204987	13.21%	1.559%
4	7.093	692	698	709	rBV	196638	314004	20.23%	2.389%
5	7.551	771	776	785	rBB	154382	246038	15.85%	1.872%
6	8.275	893	899	908	rBV	229035	382087	24.62%	2.907%
7	8.722	969	975	987	rBV	187599	318547	20.53%	2.423%
8	9.434	1090	1096	1107	rBB	183503	297512	19.17%	2.263%
9	9.963	1179	1186	1199	rBV	231526	431906	27.83%	3.286%
10	10.069	1202	1204	1209	rVB2	1410	1976	0.13%	0.015%
11	10.328	1241	1248	1257	rBB	222396	367439	23.68%	2.795%
12	10.498	1270	1277	1297	rBV	198549	415460	26.77%	3.160%
13	11.951	1521	1524	1528	rBB	2443	3299	0.21%	0.025%
14	13.639	1804	1811	1822	rBV	521600	719226	46.34%	5.471%
15	13.904	1849	1856	1865	rBV	601582	827302	53.31%	6.293%
16	14.210	1902	1908	1917	rBB	373496	535055	34.48%	4.070%
17	14.469	1947	1952	1971	rBV	134478	288202	18.57%	2.192%
18	15.216	2072	2079	2087	rBV	780504	1045990	67.40%	7.957%
19	15.380	2102	2107	2118	rBV	174485	267603	17.24%	2.036%
20	15.457	2118	2120	2124	rVB	6344	6301	0.41%	0.048%
21	16.763	2339	2342	2346	rVB3	1073	1712	0.11%	0.013%
22	16.974	2372	2378	2384	rBV2	493898	678381	43.71%	5.160%
23	17.074	2388	2395	2406	rBV	863084	1155975	74.48%	8.794%
24	18.239	2589	2593	2594	rBV	1348	1781	0.11%	0.014%
25	19.010	2721	2724	2728	rBV2	7742	9111	0.59%	0.069%
26	19.268	2763	2768	2772	rBV2	6474	8863	0.57%	0.067%
27	19.380	2781	2787	2799	rBV	1196942	1551986	100.00%	11.806%
28	21.186	3088	3094	3103	rBV	602710	845307	54.47%	6.430%
29	23.233	3435	3442	3453	rVB	690287	1251631	80.65%	9.521%
30	23.374	3460	3466	3477	rVB	379030	668079	43.05%	5.082%


Sum of corrected areas: 13145655

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022283.D
Acq On : 24 Aug 2019 07:51
Operator : HP/JU
Sample : PB122365BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

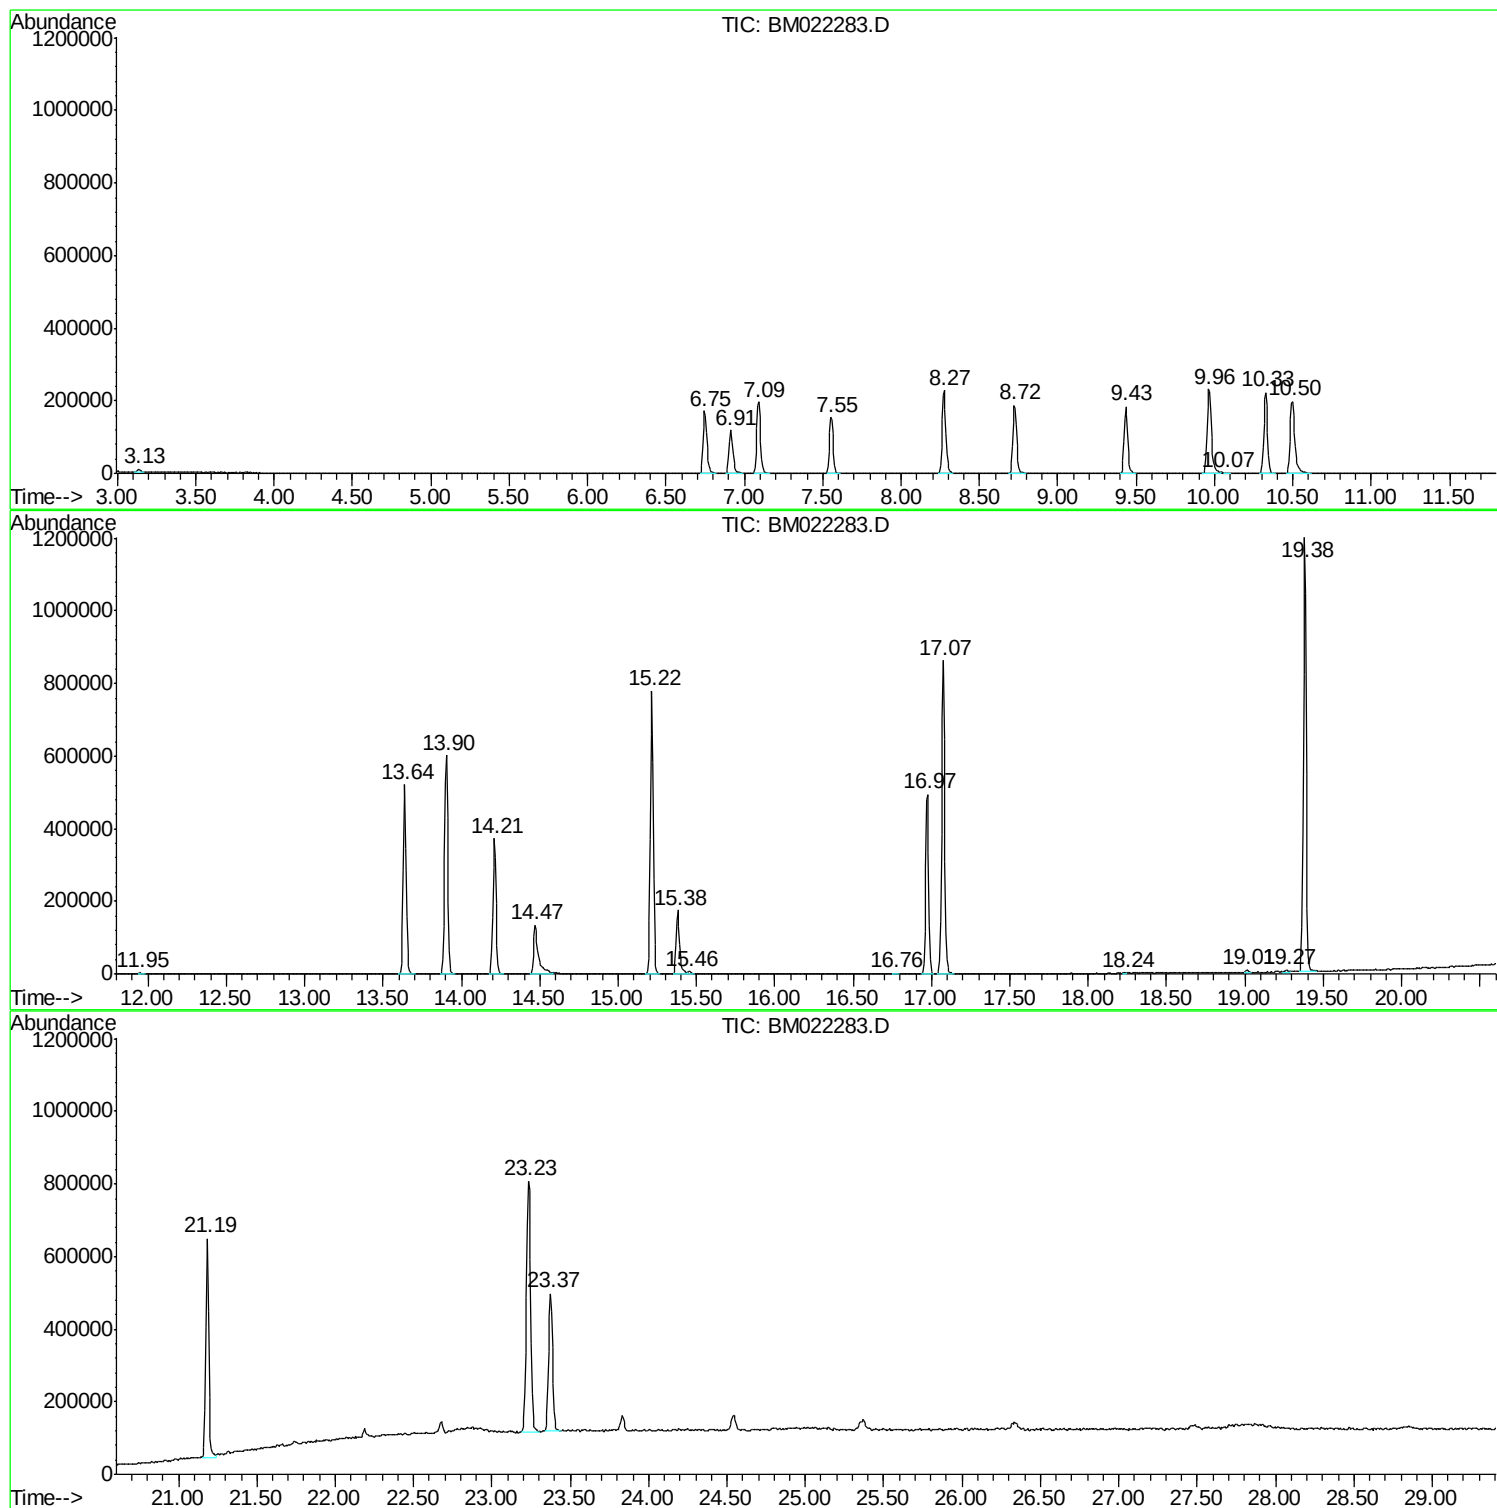

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022283.D
Acq On : 24 Aug 2019 07:51
Operator : HP/JU
Sample : PB122365BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022283.D
Acq On : 24 Aug 2019 07:51
Operator : HP/JU
Sample : PB122365BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc