

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022295.D
 Acq On : 24 Aug 2019 15:49
 Operator : HP/JU
 Sample : K4337-19DL 50X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	17	19	21	rVV2	1052	948	0.15%	0.030%
2	3.140	24	26	29	rVB3	1753	1686	0.27%	0.054%
3	3.316	52	56	57	rVB2	1171	1235	0.20%	0.039%
4	3.363	62	64	67	rVB	1310	1501	0.24%	0.048%
5	3.393	67	69	70	rBV	993	720	0.12%	0.023%
6	3.440	75	77	80	rBV3	1027	1353	0.22%	0.043%
7	3.734	125	127	128	rBV2	830	718	0.12%	0.023%
8	3.816	136	141	143	rBV	1030	1461	0.23%	0.047%
9	3.899	153	155	157	rVB2	1199	951	0.15%	0.030%
10	4.146	195	197	200	rBV2	568	744	0.12%	0.024%
11	4.246	212	214	218	rVB	794	878	0.14%	0.028%
12	4.634	277	280	283	rBV2	745	959	0.15%	0.031%
13	5.057	351	352	357	rBV	644	734	0.12%	0.023%
14	5.293	390	392	395	rVB	737	696	0.11%	0.022%
15	6.598	611	614	617	rVB	704	896	0.14%	0.029%
16	6.622	617	618	621	rBV	788	720	0.12%	0.023%
17	6.716	632	634	637	rBV	740	827	0.13%	0.026%
18	7.498	765	767	771	rBV	404	781	0.13%	0.025%
19	7.557	771	777	793	rVB	101927	175621	28.22%	5.603%
20	7.910	831	837	842	rBV3	5356	8689	1.40%	0.277%
21	8.087	862	867	871	rVB2	1482	2155	0.35%	0.069%
22	8.281	897	900	903	rVB	504	722	0.12%	0.023%
23	8.463	928	931	933	rBV	527	693	0.11%	0.022%
24	8.681	965	968	972	rBV	468	903	0.15%	0.029%
25	8.751	977	980	981	rBV	791	805	0.13%	0.026%
26	9.122	1040	1043	1047	rBV	416	898	0.14%	0.029%
27	9.645	1130	1132	1137	rBV	442	999	0.16%	0.032%
28	10.033	1195	1198	1201	rVB	754	883	0.14%	0.028%
29	10.186	1220	1224	1226	rVB	542	761	0.12%	0.024%
30	10.328	1240	1248	1252	rBV	162966	277865	44.66%	8.865%
31	10.381	1252	1257	1269	rVV	186186	336121	54.02%	10.723%
32	10.504	1272	1278	1286	rVB2	10228	17538	2.82%	0.560%
33	10.792	1322	1327	1328	rBV	464	776	0.12%	0.025%
34	11.386	1425	1428	1433	rVV	1454	1695	0.27%	0.054%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022295.D
 Acq On : 24 Aug 2019 15:49
 Operator : HP/JU
 Sample : K4337-19DL 50X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	11.439	1434	1437	1442	rVB2	1500	2328	0.37%	0.074%
36	11.969	1523	1527	1530	rBV	813	1181	0.19%	0.038%
37	12.010	1530	1534	1541	rVV	10714	18849	3.03%	0.601%
38	12.080	1543	1546	1548	rVB2	781	825	0.13%	0.026%
39	12.139	1552	1556	1560	rVV2	1764	2456	0.39%	0.078%
40	12.233	1565	1572	1578	rBB	11214	17817	2.86%	0.568%
41	12.545	1622	1625	1627	rVB	841	874	0.14%	0.028%
42	12.722	1654	1655	1658	rBV	874	846	0.14%	0.027%
43	13.022	1702	1706	1707	rBV	813	975	0.16%	0.031%
44	13.045	1707	1710	1713	rVB2	1197	1414	0.23%	0.045%
45	13.269	1746	1748	1752	rVB	430	687	0.11%	0.022%
46	13.504	1784	1788	1790	rBV	813	1117	0.18%	0.036%
47	13.651	1809	1813	1819	rBV	5074	7132	1.15%	0.228%
48	13.727	1824	1826	1831	rVB	999	1384	0.22%	0.044%
49	13.910	1851	1857	1861	rBV2	6141	9624	1.55%	0.307%
50	14.210	1902	1908	1915	rBV	287182	413866	66.51%	13.204%
51	14.280	1915	1920	1924	rVB	16568	23667	3.80%	0.755%
52	14.333	1924	1929	1930	rBV	539	846	0.14%	0.027%
53	14.392	1936	1939	1942	rBV2	991	1139	0.18%	0.036%
54	14.521	1958	1961	1965	rVB2	861	732	0.12%	0.023%
55	14.563	1965	1968	1971	rBV2	1242	1832	0.29%	0.058%
56	14.633	1976	1980	1983	rBV	2574	3696	0.59%	0.118%
57	15.221	2074	2080	2086	rBV	8279	11575	1.86%	0.369%
58	15.280	2086	2090	2094	rVB	3605	5304	0.85%	0.169%
59	15.533	2130	2133	2134	rBV	994	862	0.14%	0.028%
60	15.551	2134	2136	2138	rVB	1197	758	0.12%	0.024%
61	15.621	2145	2148	2150	rVB2	1503	1129	0.18%	0.036%
62	15.686	2156	2159	2162	rVB2	898	1138	0.18%	0.036%
63	15.998	2204	2212	2218	rVB2	6067	14806	2.38%	0.472%
64	16.198	2242	2246	2251	rVB2	1498	2285	0.37%	0.073%
65	16.257	2254	2256	2259	rBV2	1702	2731	0.44%	0.087%
66	16.545	2299	2305	2308	rVV2	1282	2204	0.35%	0.070%
67	16.668	2324	2326	2329	rBV2	1326	1400	0.22%	0.045%
68	16.762	2339	2342	2345	rVB	949	1108	0.18%	0.035%
69	16.857	2356	2358	2361	rVB2	1560	1222	0.20%	0.039%
70	16.974	2372	2378	2386	rBV2	361209	517572	83.18%	16.512%
71	17.080	2392	2396	2401	rBV	12569	15998	2.57%	0.510%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
 Data File : BM022295.D
 Acq On : 24 Aug 2019 15:49
 Operator : HP/JU
 Sample : K4337-19DL 50X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	17.257	2423	2426	2427	rBV	976	845	0.14%	0.027%
73	17.339	2439	2440	2443	rBV	1075	711	0.11%	0.023%
74	17.386	2445	2448	2449	rBV	1314	1772	0.28%	0.057%
75	17.404	2449	2451	2457	rVB	5968	7163	1.15%	0.229%
76	17.509	2466	2469	2471	rBV2	1114	1357	0.22%	0.043%
77	17.592	2481	2483	2485	rBV2	1020	806	0.13%	0.026%
78	17.745	2507	2509	2512	rVB	831	867	0.14%	0.028%
79	17.880	2528	2532	2534	rBV2	1144	1706	0.27%	0.054%
80	17.962	2543	2546	2549	rBV2	1218	1473	0.24%	0.047%
81	18.109	2567	2571	2572	rBV2	979	1169	0.19%	0.037%
82	18.233	2588	2592	2594	rBV3	1006	798	0.13%	0.025%
83	18.256	2594	2596	2600	rVB3	725	937	0.15%	0.030%
84	18.486	2631	2635	2638	rBV2	1407	1578	0.25%	0.050%
85	18.527	2638	2642	2644	rBV4	1256	1925	0.31%	0.061%
86	18.592	2649	2653	2654	rBV3	1543	1634	0.26%	0.052%
87	18.621	2657	2658	2661	rVB3	1262	775	0.12%	0.025%
88	18.686	2665	2669	2670	rBV2	1569	1345	0.22%	0.043%
89	18.780	2683	2685	2688	rVB2	1208	1079	0.17%	0.034%
90	18.809	2688	2690	2692	rBV2	1061	1040	0.17%	0.033%
91	18.903	2703	2706	2709	rBV3	1598	2489	0.40%	0.079%
92	19.080	2734	2736	2737	rBV	1373	745	0.12%	0.024%
93	19.209	2756	2758	2760	rVB3	2437	1925	0.31%	0.061%
94	19.233	2760	2762	2764	rBV2	2654	2463	0.40%	0.079%
95	19.280	2767	2770	2771	rVB3	2054	1905	0.31%	0.061%
96	19.339	2778	2780	2783	rBV4	2031	2796	0.45%	0.089%
97	19.386	2784	2788	2794	rVV2	15785	24202	3.89%	0.772%
98	19.498	2805	2807	2808	rBV2	2139	1471	0.24%	0.047%
99	21.186	3089	3094	3100	rBV	475339	622228	100.00%	19.851%
100	23.380	3461	3467	3479	rVB	267558	506971	81.48%	16.174%


Sum of corrected areas: 3134486

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082319\
Data File : BM022295.D
Acq On : 24 Aug 2019 15:49
Operator : HP/JU
Sample : K4337-19DL 50X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB6DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

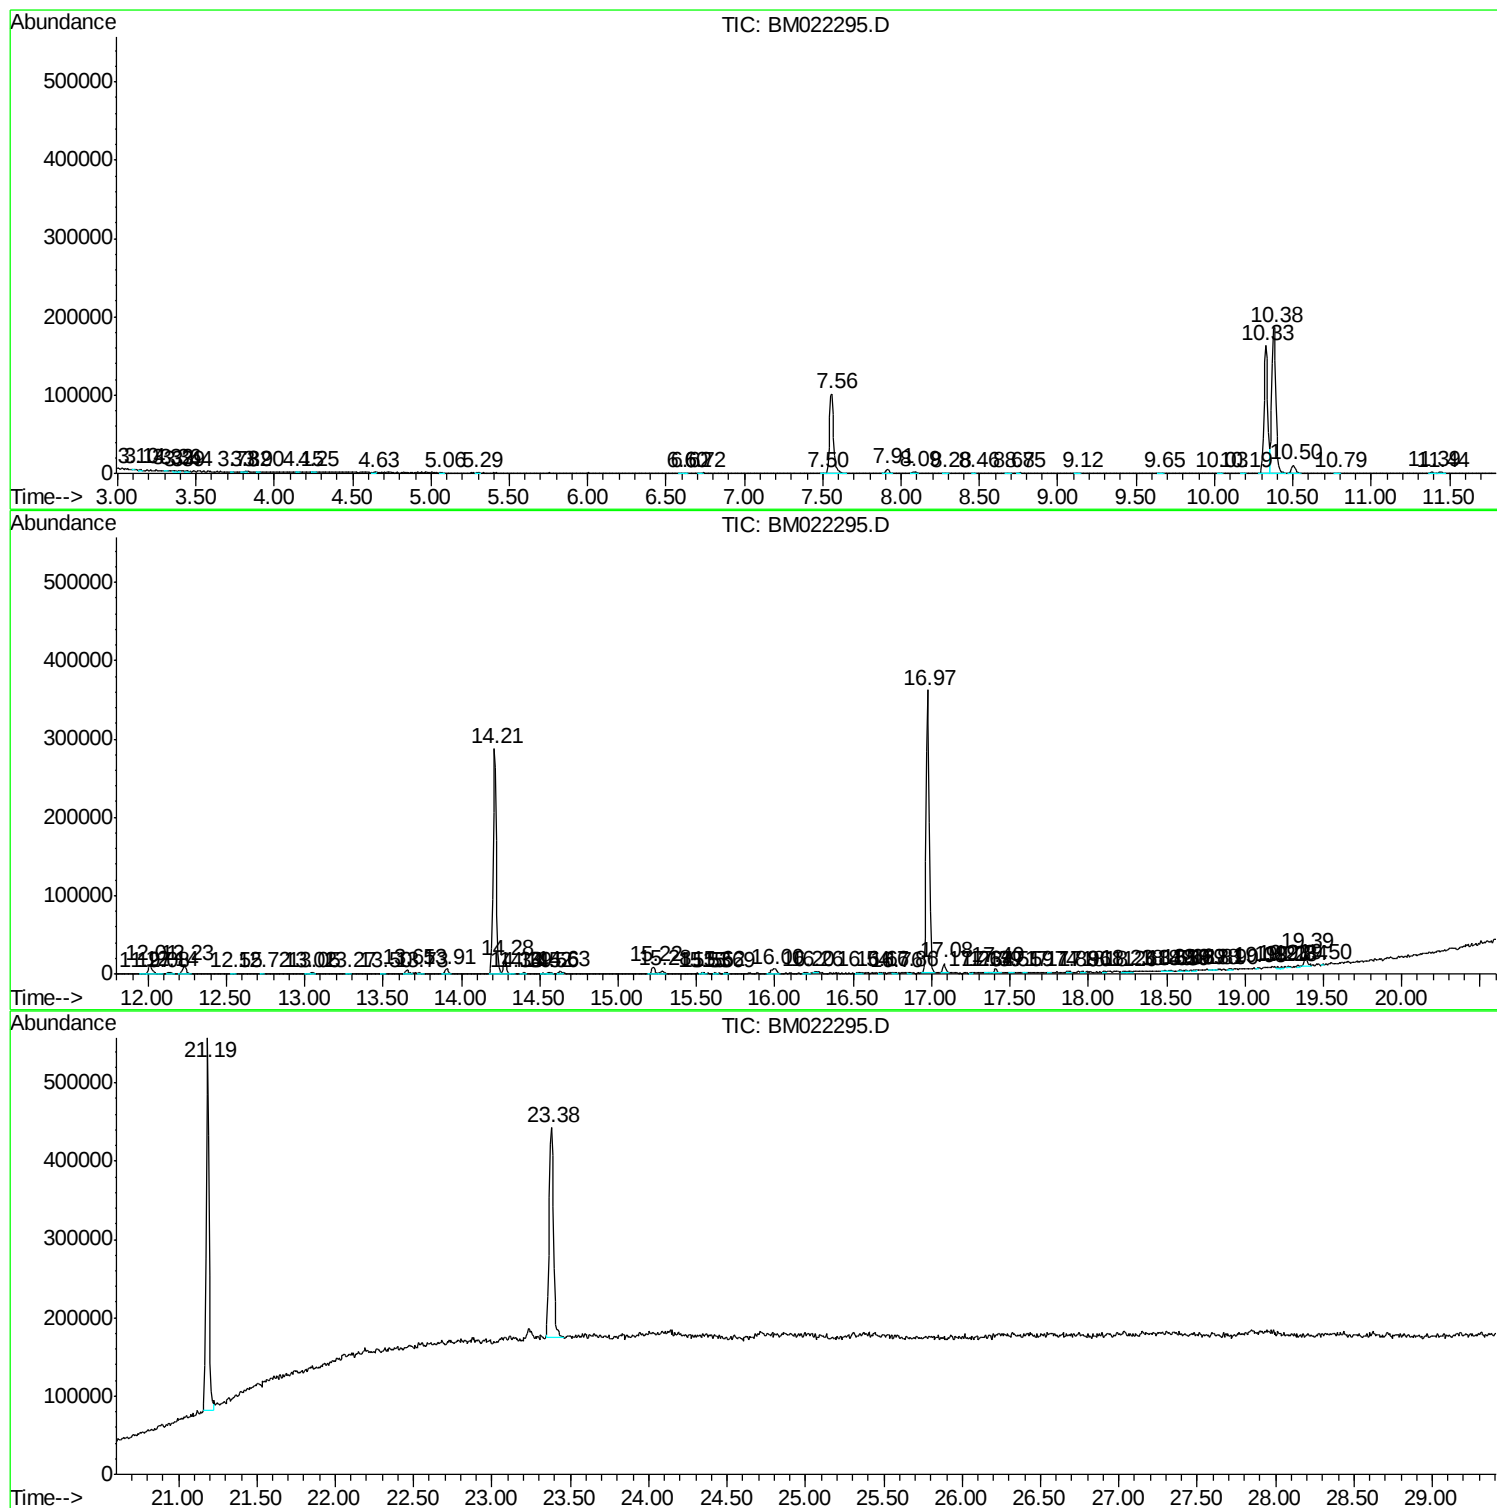

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022295.D
Acq On : 24 Aug 2019 15:49
Operator : HP/JU
Sample : K4337-19DL 50X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB6DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022295.D
Acq On : 24 Aug 2019 15:49
Operator : HP/JU
Sample : K4337-19DL 50X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB6DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc