

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
 Data File : BM022315.D
 Acq On : 25 Aug 2019 05:25
 Operator : HP/JU
 Sample : K4373-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	32	rVB	6916	9659	1.12%	0.110%
2	3.716	121	124	126	rBV2	2144	1886	0.22%	0.021%
3	3.816	138	141	144	rVB3	1774	1915	0.22%	0.022%
4	4.363	232	234	240	rBV2	626	873	0.10%	0.010%
5	4.775	303	304	308	rVB2	1015	1048	0.12%	0.012%
6	4.816	308	311	314	rBV	1131	1523	0.18%	0.017%
7	4.987	337	340	343	rBV	738	939	0.11%	0.011%
8	5.163	368	370	373	rBV	678	881	0.10%	0.010%
9	6.598	611	614	617	rBV	877	1230	0.14%	0.014%
10	6.763	636	642	653	rBB4	19022	41446	4.83%	0.470%
11	6.910	662	667	682	rBV	62905	110589	12.88%	1.255%
12	7.093	693	698	710	rBB	93875	153302	17.85%	1.739%
13	7.551	769	776	786	rVB	163552	258046	30.05%	2.927%
14	8.281	895	900	910	rBV	69363	118060	13.75%	1.339%
15	8.722	968	975	991	rBB	100615	178887	20.83%	2.029%
16	9.034	1025	1028	1032	rBB2	1791	2239	0.26%	0.025%
17	9.434	1091	1096	1105	rBV	100532	166402	19.38%	1.888%
18	9.981	1181	1189	1210	rBV	103081	251791	29.32%	2.856%
19	10.328	1241	1248	1254	rBV	237438	393405	45.82%	4.463%
20	10.534	1279	1283	1286	rBV	1794	2938	0.34%	0.033%
21	11.945	1520	1523	1526	rBB	1558	1672	0.19%	0.019%
22	13.639	1804	1811	1816	rBV	301718	453097	52.77%	5.140%
23	13.686	1816	1819	1825	rVB	17480	22997	2.68%	0.261%
24	13.898	1849	1855	1868	rBV	348884	512437	59.68%	5.813%
25	13.992	1870	1871	1876	rVB	918	1129	0.13%	0.013%
26	14.210	1902	1908	1917	rVB	401059	585074	68.14%	6.637%
27	14.527	1959	1962	1963	rBV	6082	5843	0.68%	0.066%
28	14.545	1963	1965	1969	rVB2	3575	4385	0.51%	0.050%
29	14.621	1976	1978	1982	rBV	2114	2502	0.29%	0.028%
30	14.657	1982	1984	1988	rVB	1102	1132	0.13%	0.013%
31	15.216	2072	2079	2086	rBV	427665	645733	75.20%	7.326%
32	15.269	2086	2088	2094	rVB	3044	4087	0.48%	0.046%
33	15.386	2103	2108	2117	rBV	104209	166150	19.35%	1.885%
34	15.457	2117	2120	2123	rVV2	3307	3490	0.41%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
 Data File : BM022315.D
 Acq On : 25 Aug 2019 05:25
 Operator : HP/JU
 Sample : K4373-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

35	15.916	2193	2198	2199	rBV	1564	1486	0.17%	0.017%
36	16.221	2247	2250	2253	rBV2	884	1404	0.16%	0.016%
37	16.398	2278	2280	2281	rVB	1264	862	0.10%	0.010%
38	16.439	2284	2287	2290	rBV2	1449	1771	0.21%	0.020%
39	16.492	2295	2296	2299	rVB	1127	893	0.10%	0.010%
40	16.539	2299	2304	2305	rBV	504	868	0.10%	0.010%
41	16.568	2307	2309	2312	rBV2	723	940	0.11%	0.011%
42	16.668	2324	2326	2329	rVB	834	907	0.11%	0.010%
43	16.698	2329	2331	2332	rBV2	896	871	0.10%	0.010%
44	16.710	2332	2333	2336	rVV3	1521	1747	0.20%	0.020%
45	16.733	2336	2337	2340	rVV3	1845	2321	0.27%	0.026%
46	16.763	2340	2342	2346	rVV2	1881	1967	0.23%	0.022%
47	16.804	2348	2349	2352	rVB2	1096	1158	0.13%	0.013%
48	16.886	2360	2363	2365	rVB	1183	1411	0.16%	0.016%
49	16.974	2372	2378	2388	rVV2	511157	727373	84.71%	8.252%
50	17.068	2389	2394	2405	rVV2	500692	721839	84.07%	8.189%
51	17.257	2422	2426	2429	rBV3	1332	1834	0.21%	0.021%
52	17.280	2429	2430	2434	rVB	1394	1300	0.15%	0.015%
53	17.321	2434	2437	2440	rBV2	1539	1735	0.20%	0.020%
54	17.357	2440	2443	2444	rBV	1466	1027	0.12%	0.012%
55	17.374	2444	2446	2448	rVB2	1179	890	0.10%	0.010%
56	17.410	2451	2452	2454	rBV	1536	1244	0.14%	0.014%
57	17.451	2457	2459	2462	rVB3	1938	1226	0.14%	0.014%
58	17.580	2478	2481	2482	rBV	1360	1228	0.14%	0.014%
59	17.633	2485	2490	2494	rVB3	4315	4774	0.56%	0.054%
60	17.774	2511	2514	2517	rVB2	998	1139	0.13%	0.013%
61	17.833	2520	2524	2525	rBV2	878	1017	0.12%	0.012%
62	17.868	2525	2530	2536	rBV	44077	62195	7.24%	0.706%
63	17.951	2540	2544	2546	rVV4	3219	4722	0.55%	0.054%
64	17.974	2546	2548	2549	rVB2	1957	1292	0.15%	0.015%
65	18.004	2551	2553	2555	rVB3	1374	1042	0.12%	0.012%
66	18.021	2555	2556	2558	rBV	1533	1225	0.14%	0.014%
67	18.045	2558	2560	2562	rVV3	1712	1202	0.14%	0.014%
68	18.086	2565	2567	2570	rVB4	1224	1143	0.13%	0.013%
69	18.121	2570	2573	2575	rBV3	1432	1890	0.22%	0.021%
70	18.139	2575	2576	2579	rBV3	2393	2490	0.29%	0.028%
71	18.174	2580	2582	2585	rVB3	2070	2018	0.24%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
 Data File : BM022315.D
 Acq On : 25 Aug 2019 05:25
 Operator : HP/JU
 Sample : K4373-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

72	18.233	2590	2592	2593	rBV2	1215	902	0.11%	0.010%
73	18.292	2601	2602	2606	rVB3	1643	1487	0.17%	0.017%
74	18.392	2618	2619	2622	rBV2	2094	2256	0.26%	0.026%
75	18.457	2628	2630	2633	rVB2	1473	1096	0.13%	0.012%
76	18.533	2642	2643	2644	rBV	2185	957	0.11%	0.011%
77	18.568	2647	2649	2651	rVV2	2692	2301	0.27%	0.026%
78	18.621	2655	2658	2659	rBV	1508	1262	0.15%	0.014%
79	18.651	2661	2663	2665	rBV3	2236	2286	0.27%	0.026%
80	18.692	2668	2670	2671	rVB	1470	961	0.11%	0.011%
81	18.704	2671	2672	2673	rBV	1702	1050	0.12%	0.012%
82	18.786	2683	2686	2688	rBV4	4136	4232	0.49%	0.048%
83	19.015	2721	2725	2728	rBV3	8131	12902	1.50%	0.146%
84	19.157	2745	2749	2753	rBV3	20717	27811	3.24%	0.316%
85	19.268	2763	2768	2770	rBV	5220	6541	0.76%	0.074%
86	19.380	2781	2787	2792	rBV	662520	858648	100.00%	9.741%
87	19.462	2799	2801	2803	rVB3	2980	1835	0.21%	0.021%
88	19.692	2838	2840	2841	rBV2	3745	2253	0.26%	0.026%
89	19.909	2874	2877	2880	rBV2	13732	15885	1.85%	0.180%
90	20.409	2959	2962	2965	rBV2	19446	22366	2.60%	0.254%
91	20.874	3038	3041	3046	rBV3	50870	61615	7.18%	0.699%
92	21.180	3088	3093	3101	rBV	570120	709200	82.59%	8.046%
93	21.309	3112	3115	3120	rVB	39765	41667	4.85%	0.473%
94	21.733	3184	3187	3190	rBV2	45028	47541	5.54%	0.539%
95	22.180	3261	3263	3269	rVB	50532	55935	6.51%	0.635%
96	23.233	3435	3442	3450	rVB	343317	683050	79.55%	7.749%
97	23.374	3460	3466	3472	rVB	313543	577467	67.25%	6.551%


Sum of corrected areas: 8814744

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
Data File : BM022315.D
Acq On : 25 Aug 2019 05:25
Operator : HP/JU
Sample : K4373-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

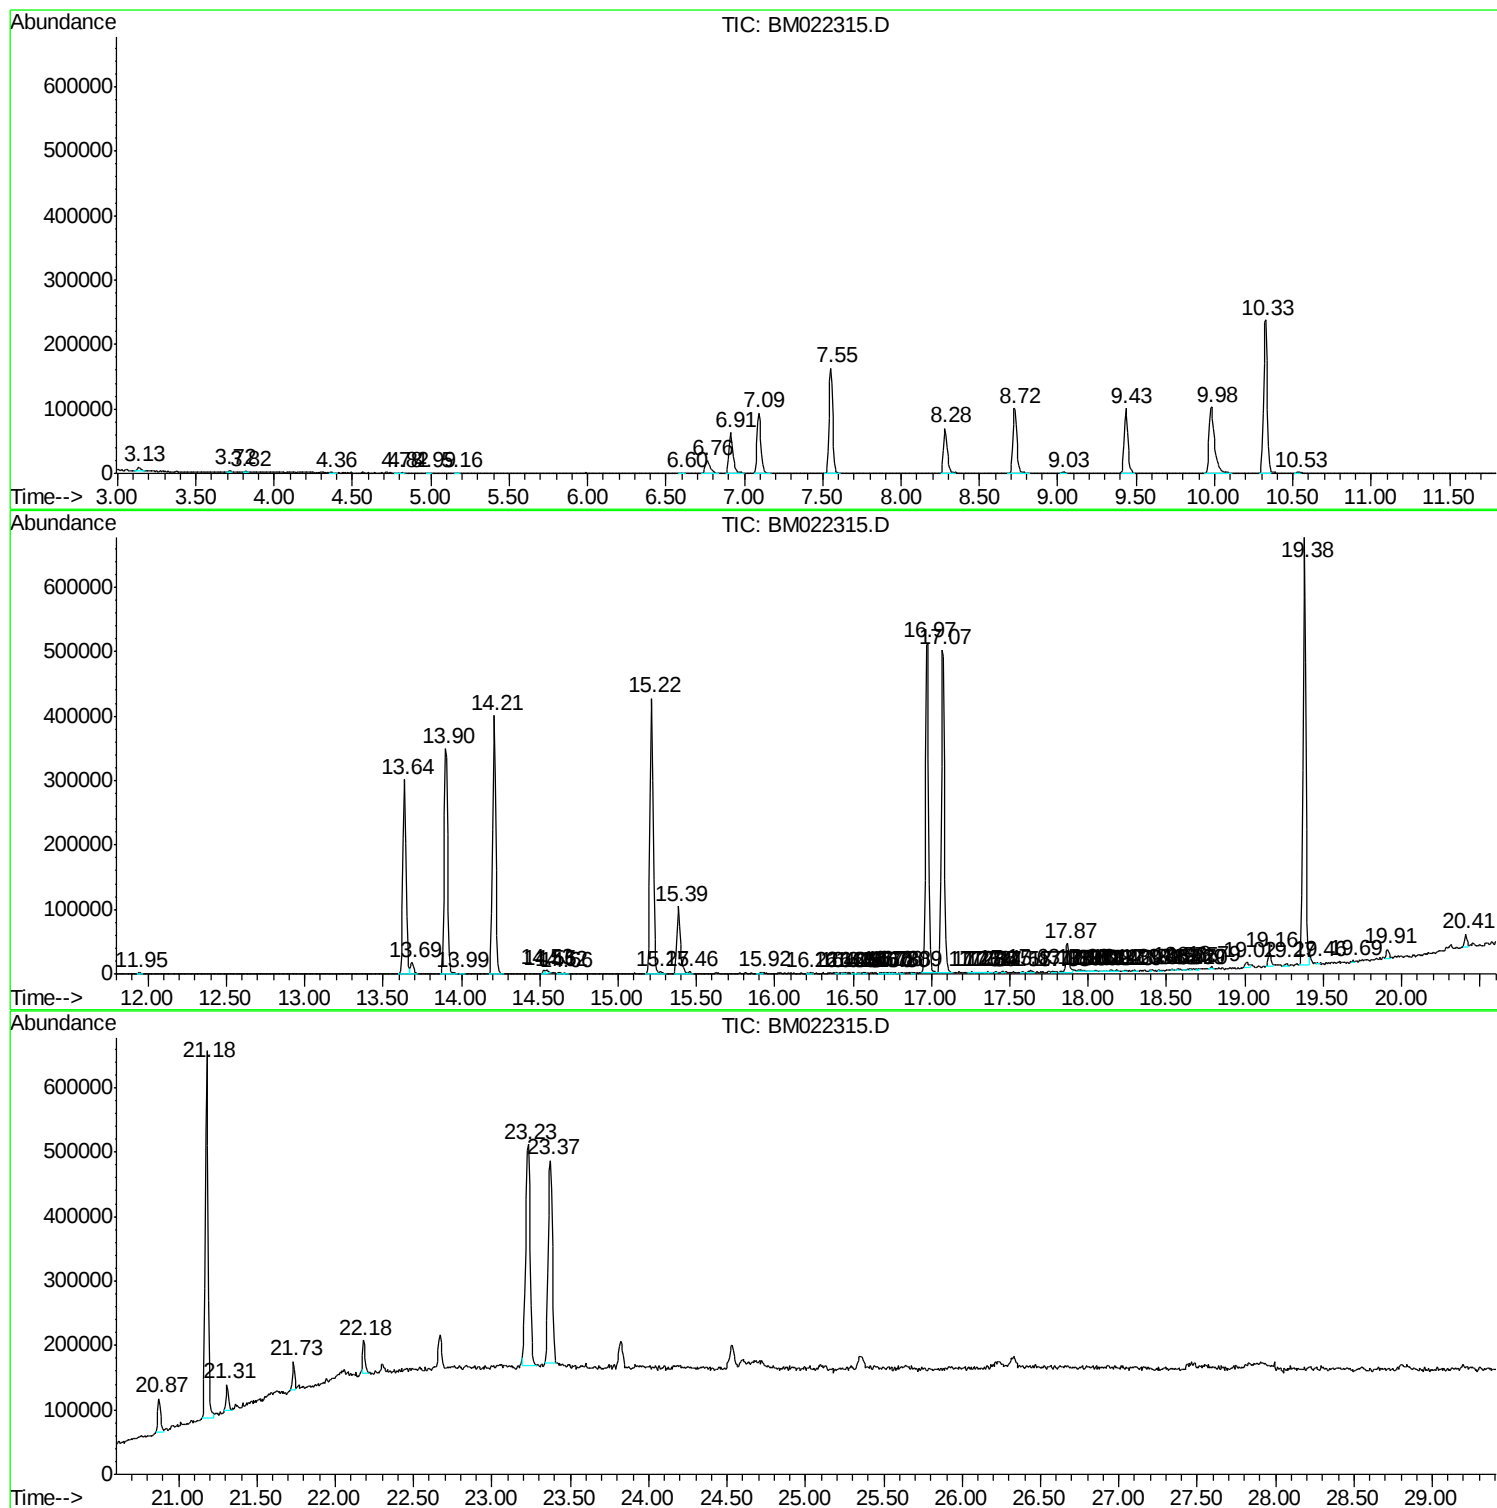

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
Data File : BM022315.D
Acq On : 25 Aug 2019 05:25
Operator : HP/JU
Sample : K4373-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082319\
Data File : BM022315.D
Acq On : 25 Aug 2019 05:25
Operator : HP/JU
Sample : K4373-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc