

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
 Data File : BM022321.D
 Acq On : 25 Aug 2019 09:04
 Operator : HP/JU
 Sample : PB122641BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	22	24	33	rVB	7582	10833	0.74%	0.085%
2	3.816	138	141	144	rBV4	1424	1588	0.11%	0.012%
3	4.910	323	327	331	rBV4	2400	3517	0.24%	0.028%
4	6.746	634	639	657	rBV	168585	298101	20.40%	2.346%
5	6.910	661	667	676	rBV	123134	198616	13.59%	1.563%
6	7.087	691	697	709	rVB	199309	322031	22.03%	2.534%
7	7.551	769	776	785	rVB	142086	235457	16.11%	1.853%
8	7.898	829	835	840	rBV3	3518	4683	0.32%	0.037%
9	8.269	892	898	911	rBV	225920	388399	26.57%	3.056%
10	8.722	968	975	985	rBV	186592	315907	21.61%	2.486%
11	9.428	1089	1095	1110	rVB	174891	297964	20.39%	2.345%
12	9.963	1180	1186	1203	rBV	227879	434321	29.72%	3.418%
13	10.322	1241	1247	1256	rVB	226604	356319	24.38%	2.804%
14	10.492	1270	1276	1295	rBV	201652	417737	28.58%	3.287%
15	11.945	1519	1523	1528	rVB2	2486	3894	0.27%	0.031%
16	13.633	1804	1810	1822	rBV	523891	725170	49.62%	5.706%
17	13.898	1849	1855	1865	rBV	596322	836276	57.22%	6.581%
18	14.204	1901	1907	1915	rVB	360937	534285	36.56%	4.204%
19	14.480	1948	1954	1979	rBV	93107	254072	17.38%	1.999%
20	15.210	2072	2078	2090	rBV	754808	1054829	72.17%	8.301%
21	15.380	2101	2107	2118	rBV	151222	244379	16.72%	1.923%
22	15.451	2118	2119	2122	rVB3	6145	4786	0.33%	0.038%
23	16.757	2337	2341	2347	rVB2	1144	1683	0.12%	0.013%
24	16.968	2371	2377	2385	rBV2	522730	681267	46.61%	5.361%
25	17.068	2388	2394	2408	rBV	849202	1204210	82.39%	9.476%
26	17.939	2539	2542	2544	rBV3	1228	1546	0.11%	0.012%
27	18.145	2572	2577	2578	rBV2	1344	1559	0.11%	0.012%
28	18.268	2595	2598	2602	rVV3	895	1843	0.13%	0.015%
29	18.827	2690	2693	2694	rBV4	1266	1542	0.11%	0.012%
30	19.009	2721	2724	2731	rBV	8032	10799	0.74%	0.085%
31	19.262	2765	2767	2770	rBV2	4990	5076	0.35%	0.040%
32	19.380	2781	2787	2800	rBV	1079968	1461565	100.00%	11.501%
33	21.180	3088	3093	3102	rBV	503897	706491	48.34%	5.560%
34	23.233	3435	3442	3450	rBV	592014	1105821	75.66%	8.702%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022321.D
Acq On : 25 Aug 2019 09:04
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Title : SVOA CALIBRATION

35	23.374	3460	3466	3474	rBV2	306088	581248	39.77%	4.574%
----	--------	------	------	------	------	--------	--------	--------	--------


Sum of corrected areas: 12707814

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022321.D
Acq On : 25 Aug 2019 09:04
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

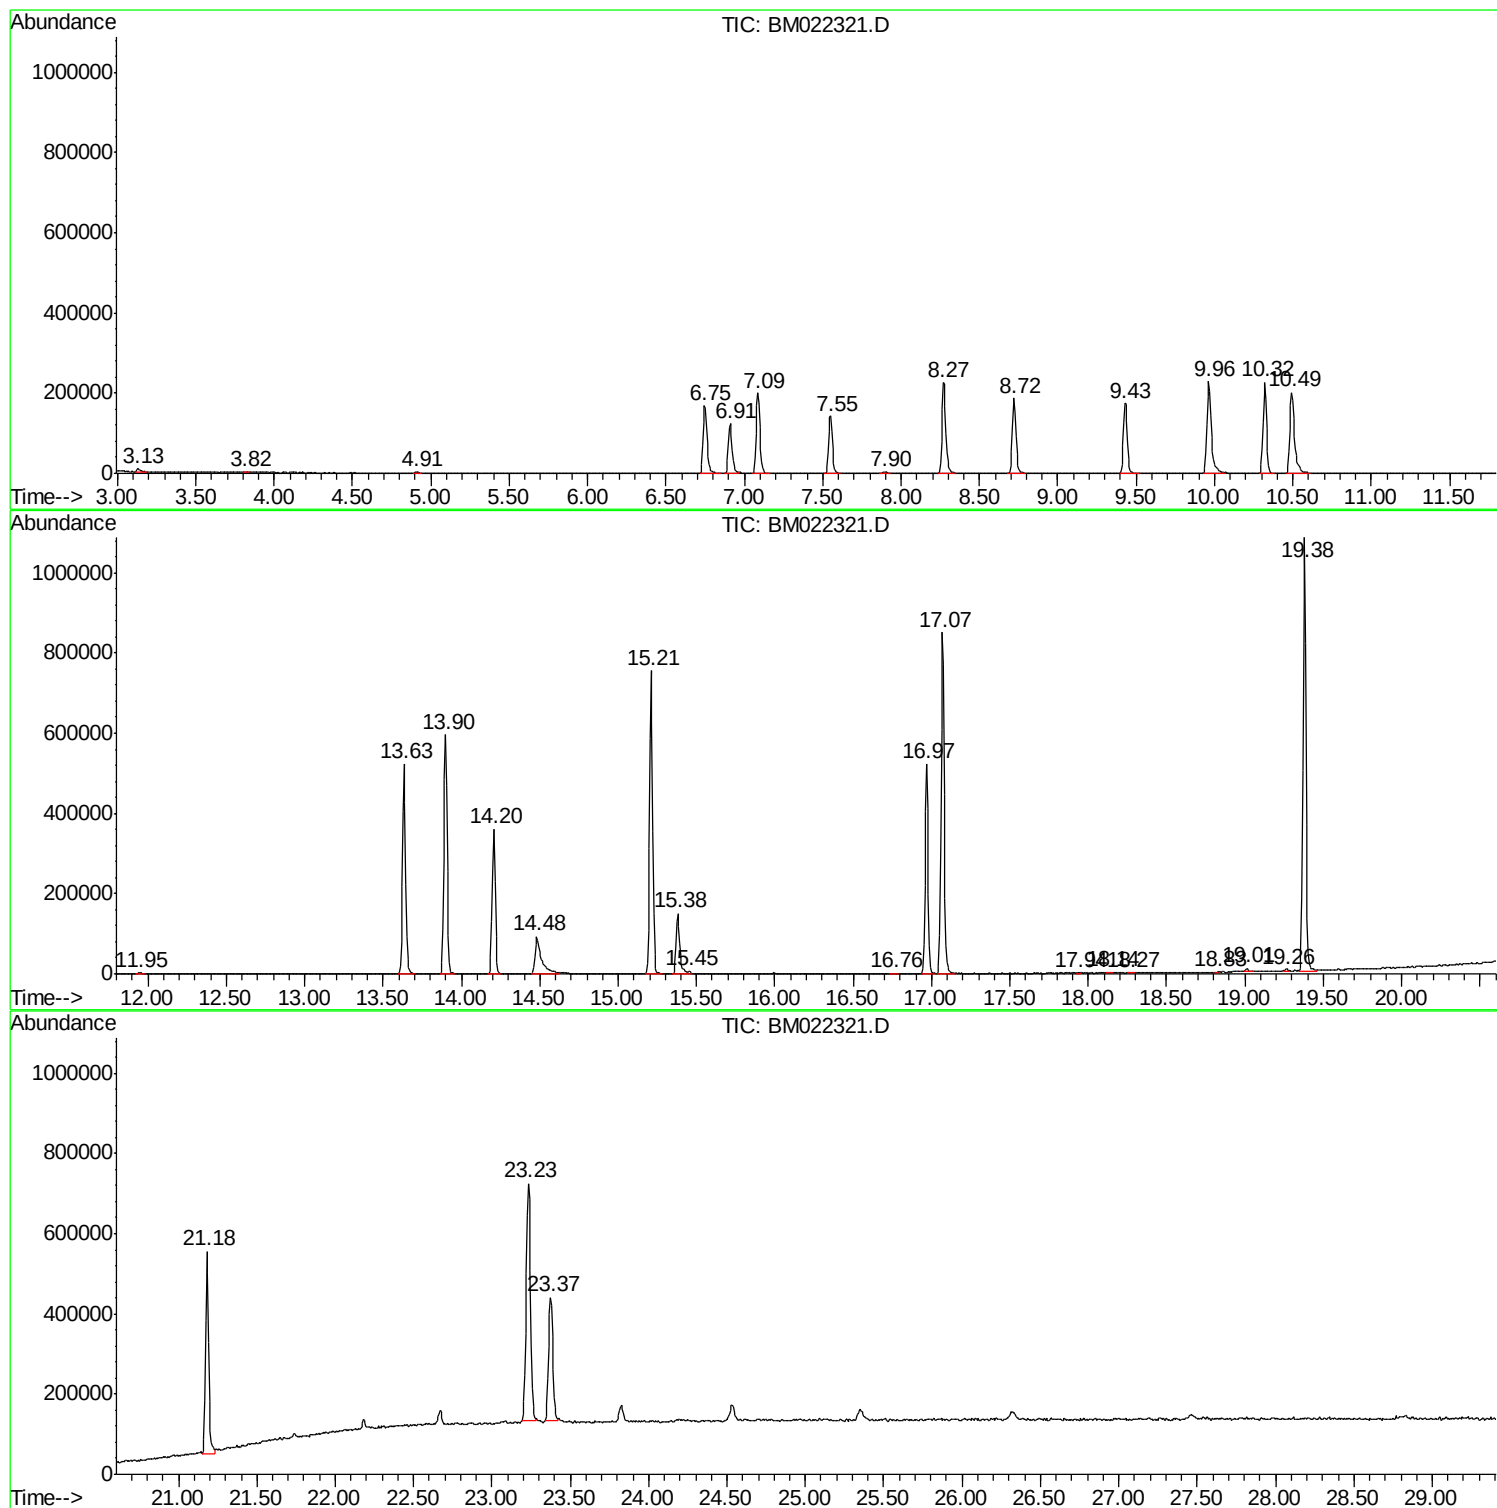

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022321.D
Acq On : 25 Aug 2019 09:04
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082319\
Data File : BM022321.D
Acq On : 25 Aug 2019 09:04
Operator : HP/JU
Sample : PB122641BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK41

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM082219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc