
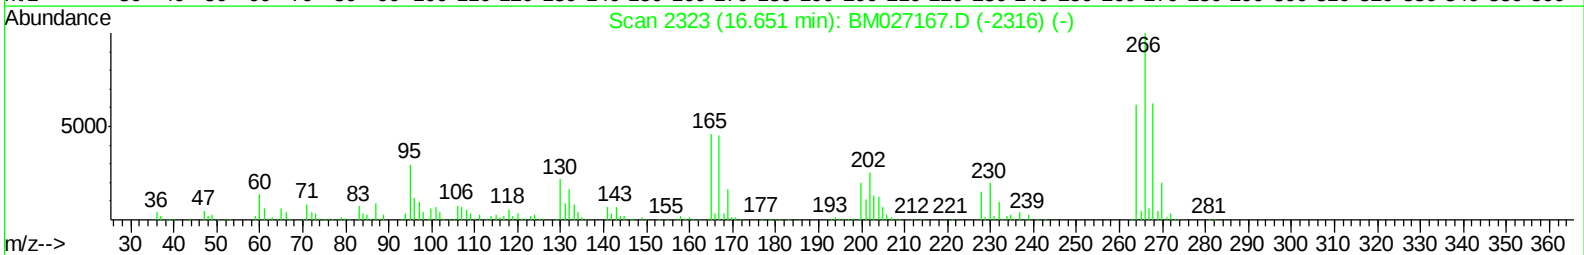
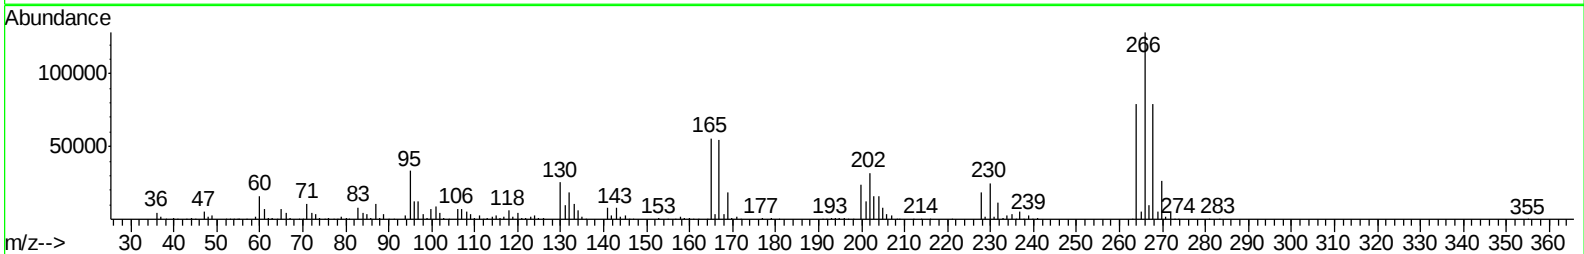


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082420\
Data File : BM027193.D
Acq On : 24 Aug 2020 13:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:49:52 2020
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 15:18:39 2020
Response via : Initial Calibration

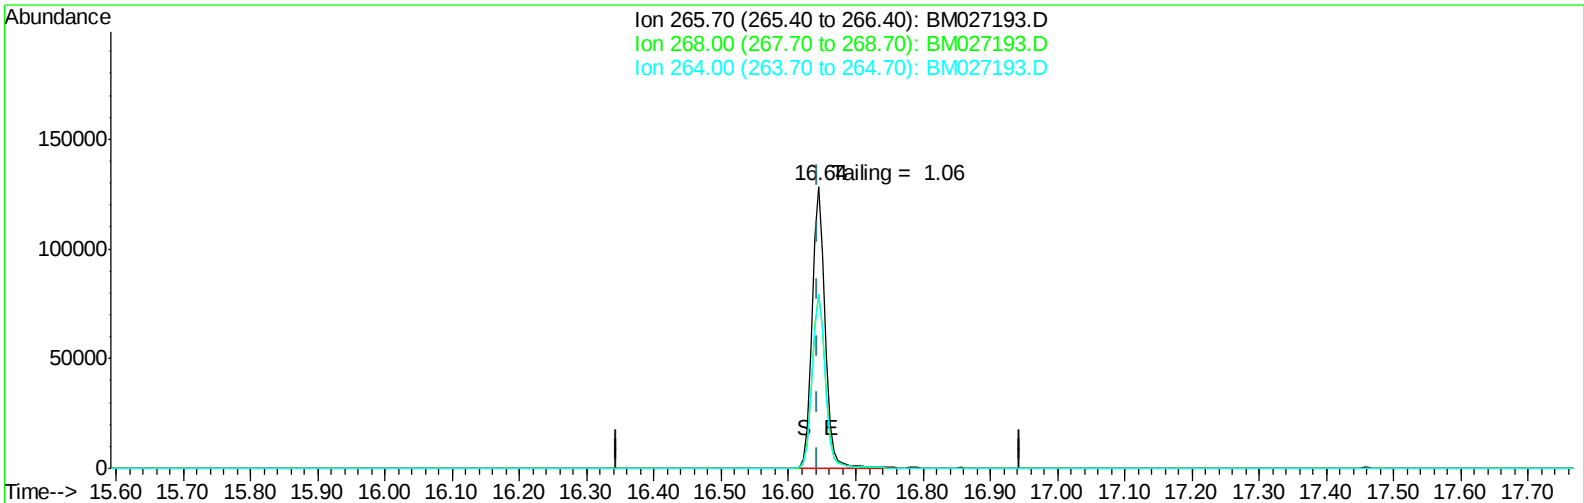

TIC: BM027193.D

(70) Pentachlorophenol (C)




16.645min (+0.000) 0.00ng

response 178265

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	62.02
264.00	61.40	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082420\
Data File : BM027193.D
Acq On : 24 Aug 2020 13:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:49:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 15:18:39 2020
Response via : Initial Calibration

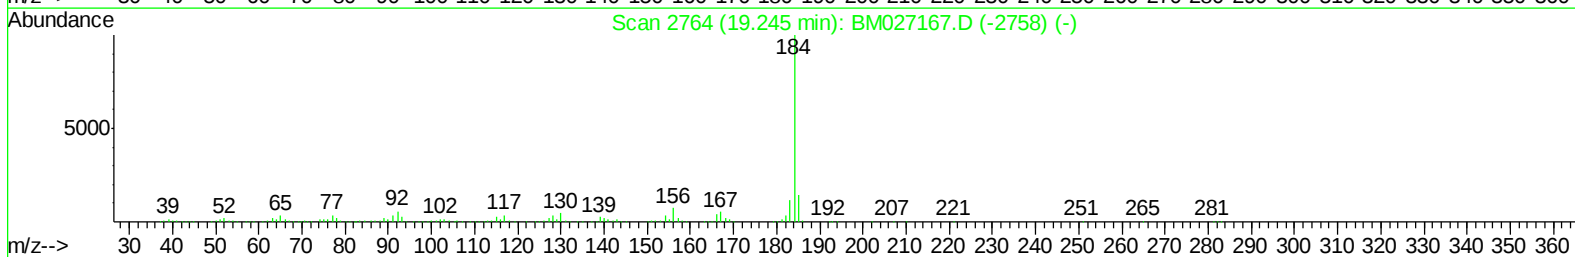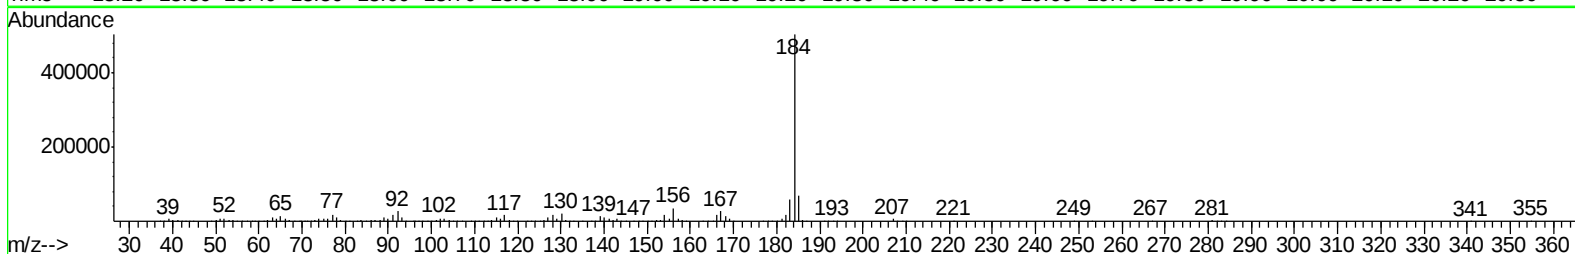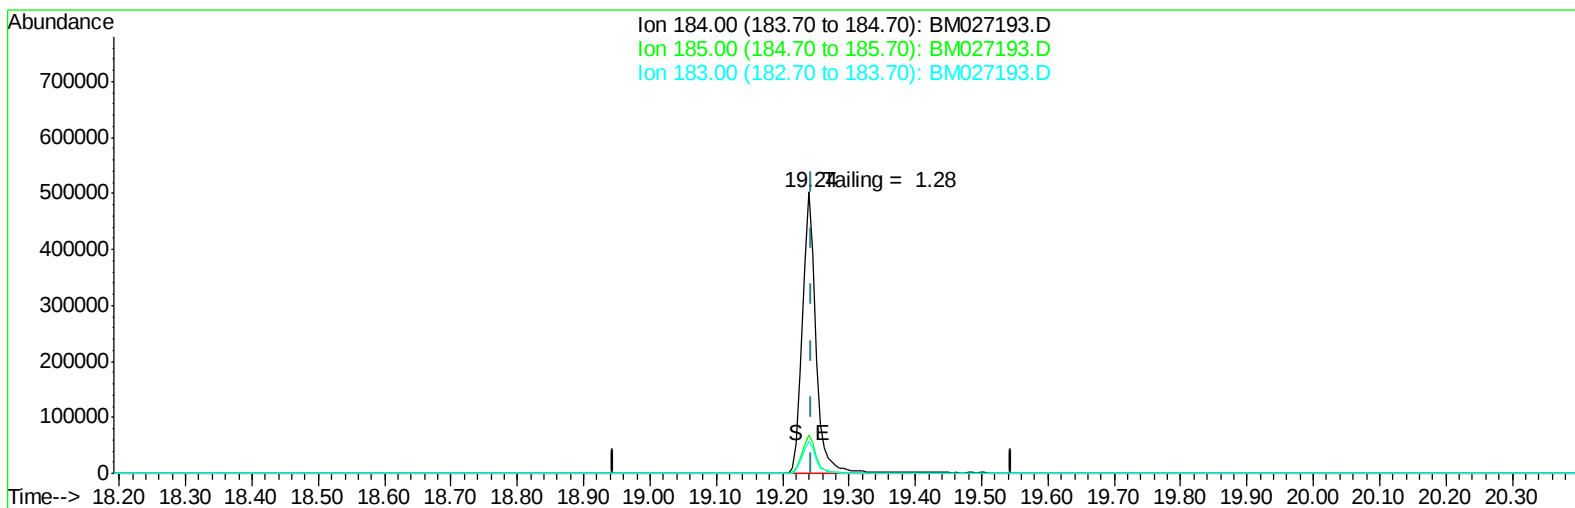

TIC: BM027193.D

(77) Benzidine

19.239min (-0.006) 94255.50ng

response 703022

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.58
183.00	11.70	11.53
0.00	0.00	0.00