


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082420\
 Data File : BM027193.D
 Acq On : 24 Aug 2020 13:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 15:18:39 2020

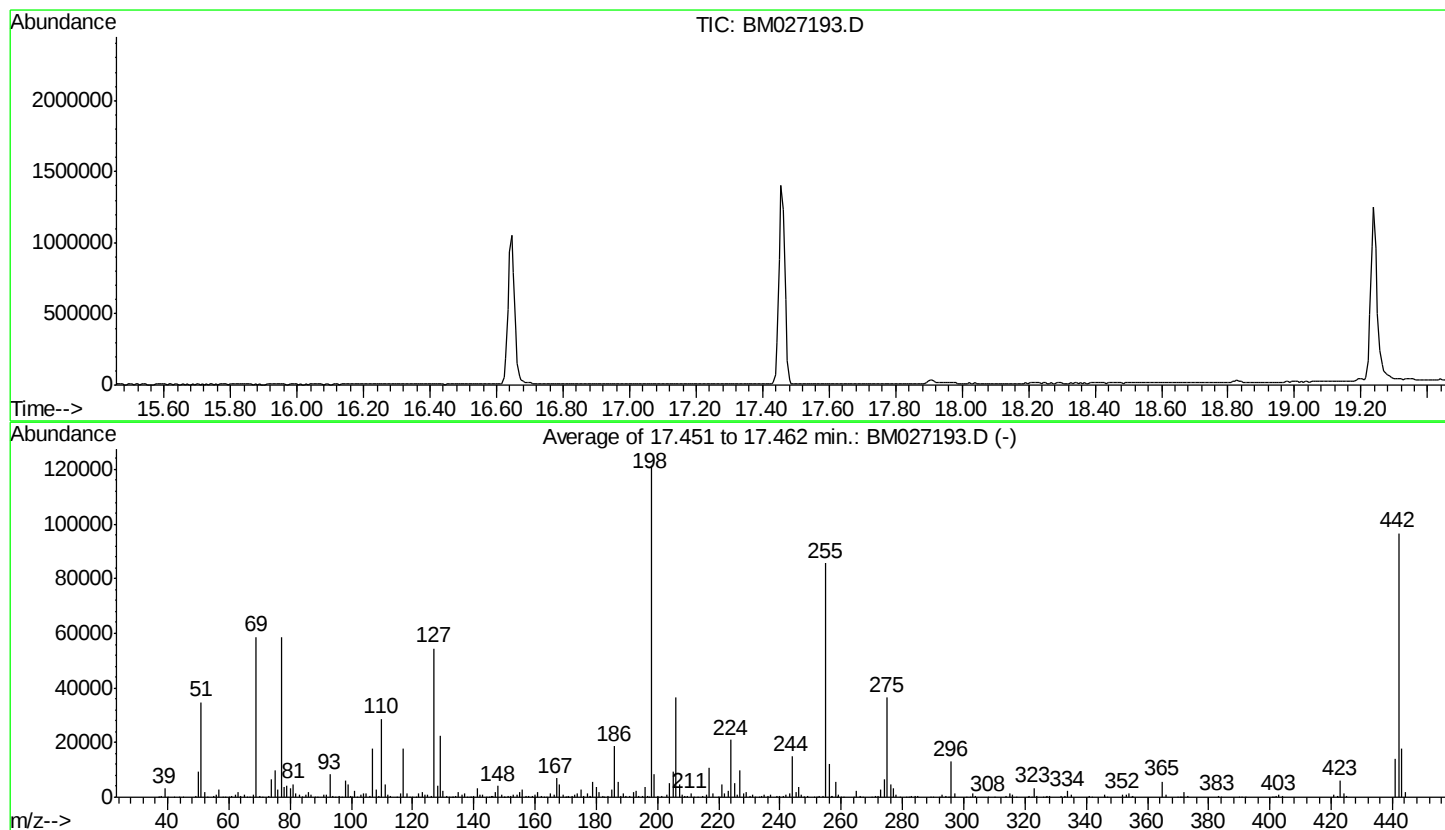

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	34785	PASS
68	69	0.00	2	1.8	1046	PASS
69	198	0.00	100	48.4	58697	PASS
70	69	0.00	2	0.5	317	PASS
127	198	10	80	45.0	54570	PASS
197	198	0.00	2	0.6	714	PASS
198	198	100	100	100.0	121370	PASS
199	198	5	9	7.0	8514	PASS
275	198	10	60	30.1	36541	PASS
365	198	1	100	4.8	5778	PASS
441	198	0.01	100	11.6	14117	PASS
442	198	50	100	79.7	96680	PASS
443	442	15	24	18.5	17905	PASS