

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
 Data File : BM041465.D
 Acq On : 24 Aug 2023 14:55
 Operator : MA/JU
 Sample : PB155026BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK026

Quant Time: Aug 24 18:36:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 24 18:34:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.118	152	11579	0.400	ng/ul	0.00
4) Naphthalene-d8	10.950	136	33079	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.759	164	15393	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.515	188	27130	0.400	ng/ul	0.00
17) Chrysene-d12	21.705	240	8138	0.400	ng/ul	0.00
23) Perylene-d12	24.281	264	10195	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.448	96	65949	4.500	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.528	152	10637	0.243	ng/ul	0.00
18) Fluoranthene-d10	19.534	212	12263	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.905	202	3484	0.046	ng/ul#	1
26) Benzo(a)pyrene	24.117	252	5930	0.103	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082423\
Data File : BM041465.D
Acq On : 24 Aug 2023 14:55
Operator : MA/JU
Sample : PB155026BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK026

Quant Time: Aug 24 18:36:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM082423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 24 18:34:12 2023
Response via : Initial Calibration




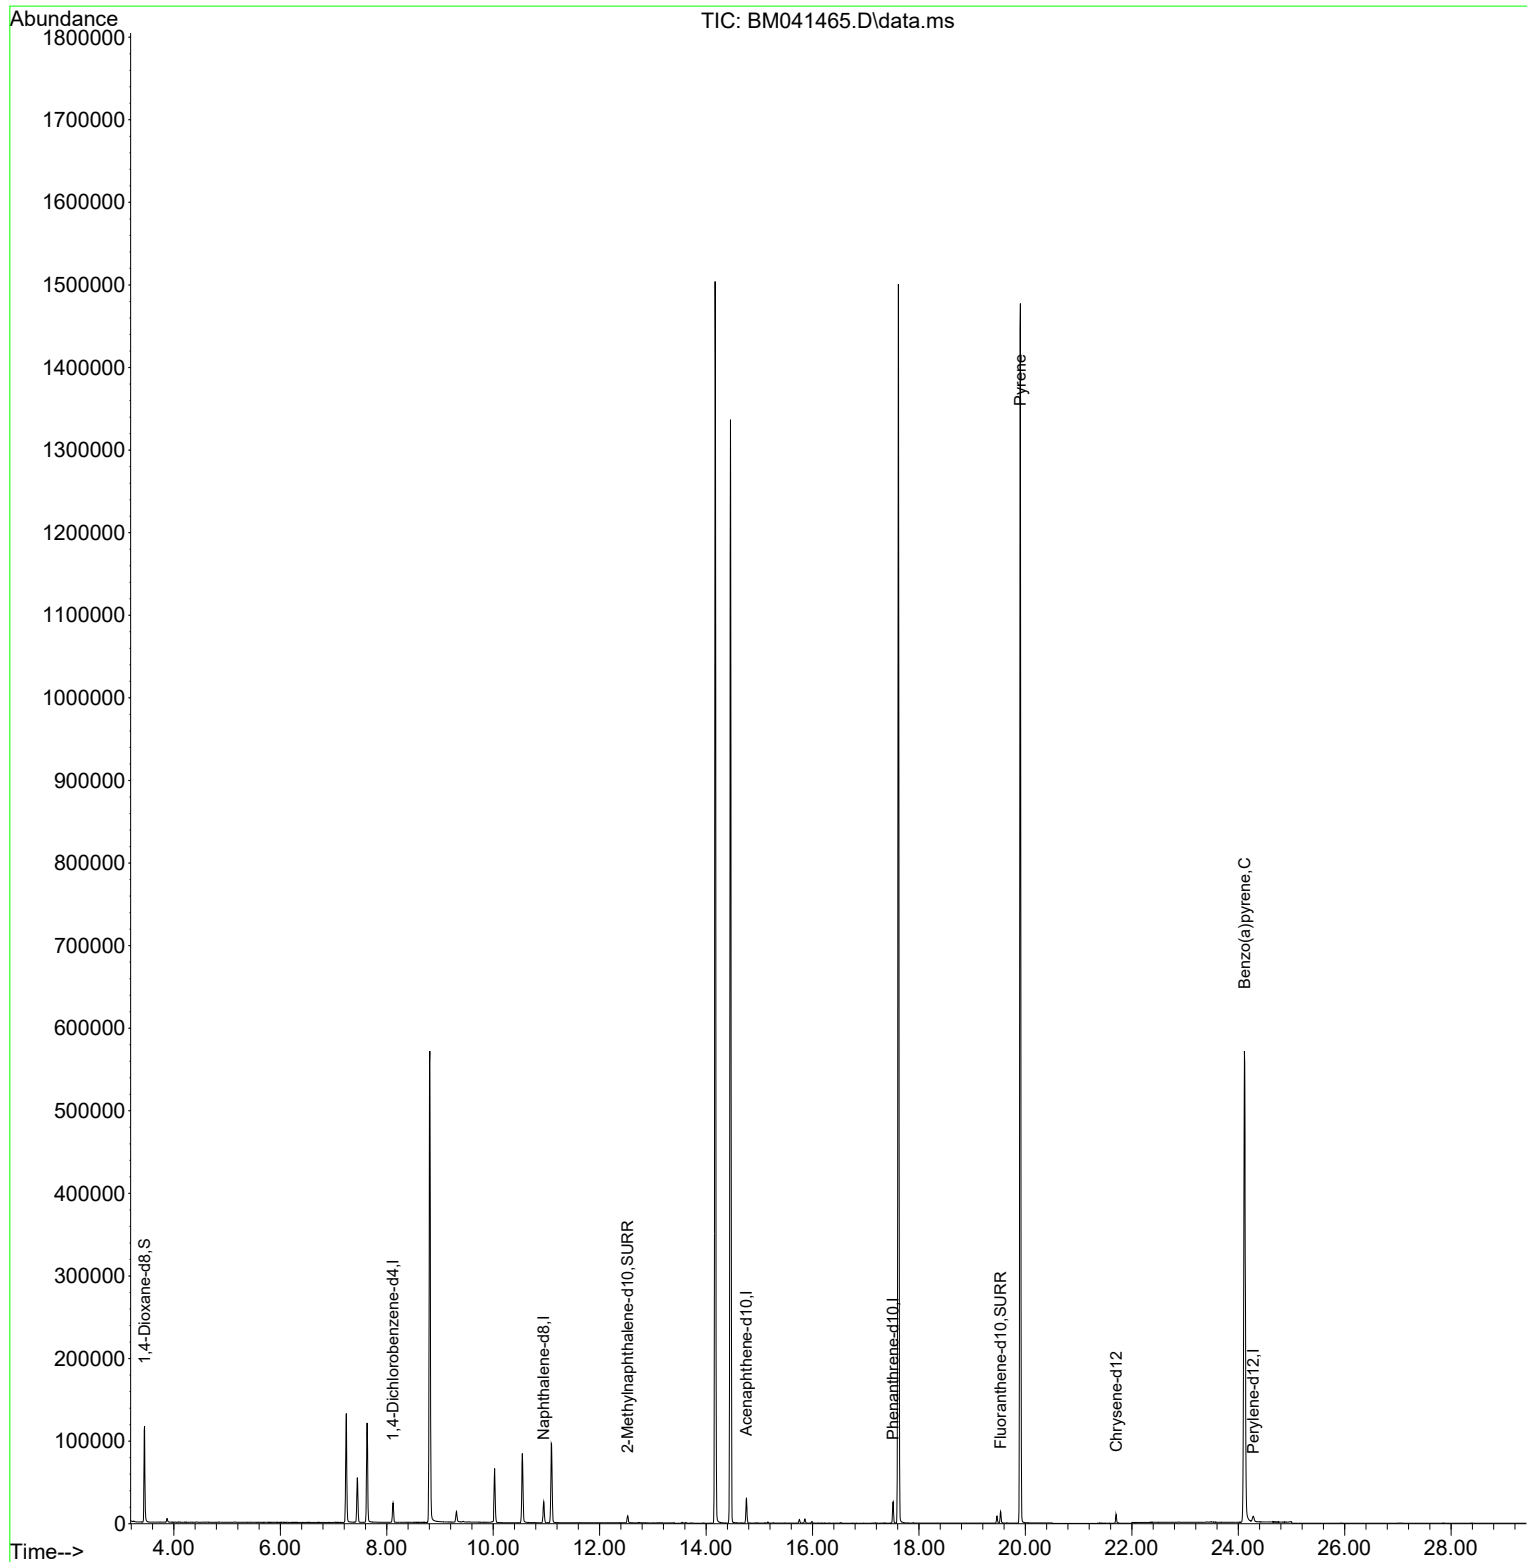


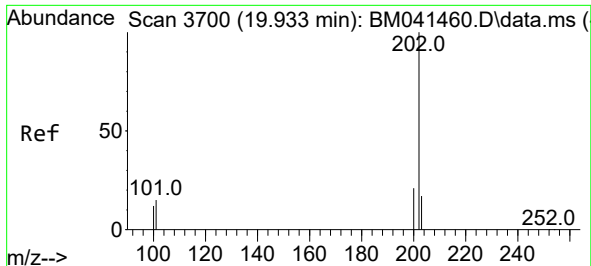

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.905 min Scan# 3
Delta R.T. -0.028 min
Lab File: BM041465.D
Acq: 24 Aug 2023 14:55

Instrument :
BNA_M
ClientSampleId :
SBLK026

Tgt Ion:202 Resp: 3484
Ion Ratio Lower Upper
202 100
101 141.1 12.2 18.2#
100 1002.4 9.8 14.8#

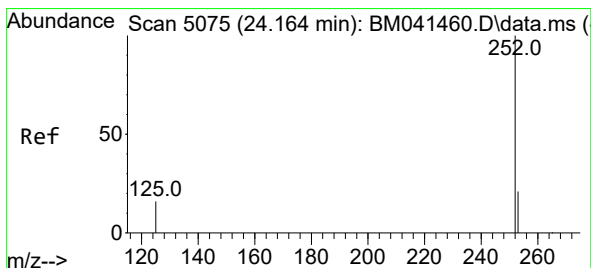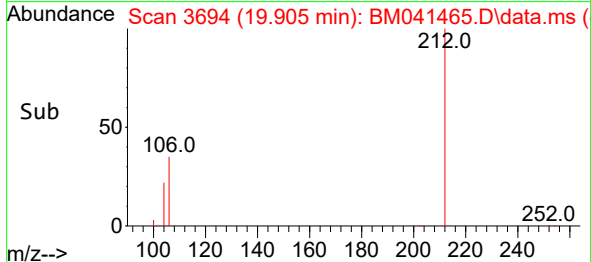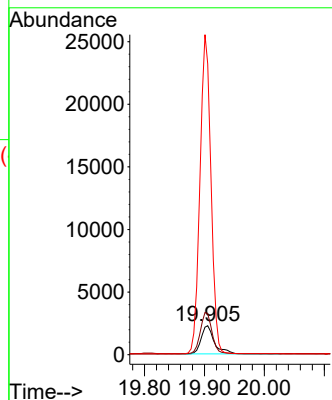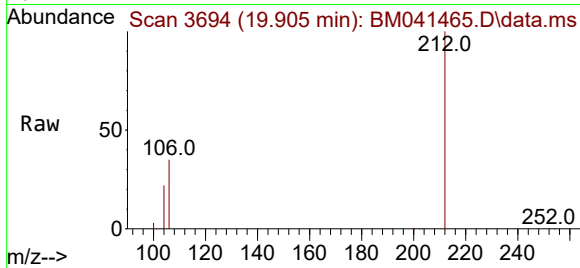

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 24.117 min Scan# 5059
Delta R.T. -0.047 min
Lab File: BM041465.D
Acq: 24 Aug 2023 14:55

Tgt Ion:252 Resp: 5930
Ion Ratio Lower Upper
252 100
253 35.8 19.5 29.3#
125 30.1 16.0 24.0#

